

Cover Sheet for

ENVIRONMENTAL CHEMISTRY METHOD

Pesticide Name: Fludioxinil (Cga-173506)

MRID #: 443823-14

Matrix: Soil

Analysis: HPLC/UV

This method is provided to you by the Environmental Protection Agency's (EPA) Environmental Chemistry Laboratory (ECL). This method is *not* an EPA method but one which was submitted to EPA by the pesticide manufacturer to support product registration. EPA recognizes that the methods may be of some utility to state, tribal, and local authorities, but makes no claim of validity by posting these methods. Although the Agency reviews *all* Environmental Chemistry Methods submitted in support of pesticide registration, the ECL evaluates only about 30% of the currently available methods. Most methods perform satisfactorily but some, particularly the older methods, have deficiencies. Moreover, the print quality of the methods varies considerably because the methods originate from different sources. Therefore, the methods offered represent the best available copies.

If you have difficulties in downloading the method, or further questions concerning the methods, you may contact Elizabeth Flynt at 228-688-2410 or via e-mail at flynt.elizabeth@epa.gov.

COLLECTOR'S LOG

THE 1970 EMISSIONS INVENTORY

GENERAL INFORMATION

PERIOD: 1970

LOCATION: NEW YORK

VACUUM: 10⁻³

(A) I measured the following materials using the method described above:
1. Polystyrene (PS) - A sample was taken from a large block of PS which
was being stored at -20°C in a vacuum desiccator. The sample was cut into
a rectangular shape, weighed, and placed in a vacuum desiccator along with
a piece of aluminum foil which was folded over the sample. A thin film of
hexane was applied to the surface of the aluminum foil. After the sample
had been heated to 100°C for 10 minutes, the sample was removed and
placed in a vacuum desiccator. After the sample had cooled to room temperature,
it was weighed again. The sample had lost approximately 3% weight.
The sample was then placed in a vacuum desiccator and left to stand for 10 minutes.
After this time, the sample was weighed again. The sample had lost an additional
3% weight. The sample was then placed in a vacuum desiccator and left to stand for
an additional 10 minutes. The sample had lost an additional 3% weight.



Columbia, Missouri

ANALYTICAL METHOD

Analysis of Soil for
CGA-339833, CGA-192155, CGA-265378, and CGA-173506

ABC METHOD NUMBER

CGA011696/Soil

AUTHOR AND DEVELOPER OF METHOD

Michael E. Gresham
ABC Laboratories
7200 ABC Lane
Columbia, MO 65202

Date January 16, 1996

Revision number 05

Revision date November 5, 1996

SPONSOR

Ciba Crop Protection
Ciba-Geigy Corporation
410 Swing Road
Greensboro, NC 27409

PERFORMING LABORATORY

Analytical Bio-Chemistry Laboratories, Inc.
7200 East ABC Lane
Columbia, Missouri 65202

Page 1 of 101

ABC Laboratories California
32380 Avenue 10
Macatawa, CA 93638 USA
Tel: 209/675-0889 Fax: 209/675-0884

ABC Laboratories Missouri
7200 E. ABC Lane
Columbia, MO 65202 USA
Tel: 573/474-8579 Fax: 573/443-9033

ABC Laboratories Europe
38 Castlewood Road
Coleraine, N. Ireland BT51 3RL
Tel: 44 (01265) 320639 Fax: 44 (01265) 320553

TABLE OF CONTENTS

	Page
TITLE PAGE	1
TABLE OF CONTENTS	2
LIST OF TABLES AND FIGURES	3
I. INTRODUCTION/SUMMARY	8
A. Scope	8
B. Principle	8
II. MATERIALS AND METHODS	8
A. Apparatus	8
B. Reagents and Analytical Standards	9
C. Reagent Solutions and Mixtures	10
D. HPLC Columns and Supplies	11
E. Safety and Health	12
F. Standard Solutions	12
G. Sample Extraction	13
H. HPLC Chromatography (General Discussion)	16
I. HPLC Analysis of CGA-265378 and CGA-173506 (non-polar analytes)	17
J. HPLC Analysis of CGA-339833 and CGA-192155 (polar analytes)	19
K. Modifications and Potential Problems	22
L. Data Acquisition and Calculations	25
III. RESULTS AND DISCUSSION	27
IV. CONCLUSIONS	28
V. CERTIFICATION	29
VI. CERTIFICATION OF GOOD LABORATORY PRACTICES	30
VII. QUALITY ASSURANCE STATEMENT	31
VIII. TABLES AND FIGURES	32
IX. REFERENCES	101

LIST OF TABLES AND FIGURES

<u>Tables</u>		<u>Page</u>
I.	Soil Characterization Data	32
II.	Calibration and Recovery Data for New Jersey Soil	33
III.	Calibration and Recovery Data for Georgia Soil	37
IV.	Summary Data for Fortified Soils	41

<u>Figures</u>		<u>Page</u>
1.	Chemical Structures	45
2.	Extraction and Analysis Scheme	47
3.	Hydraulic Schematic for the HPLC System Used in ABC Method # CGA011696	48
4.	Example Chromatogram of Analytes on a SB-CN Column Using 40% ACN: 60% Reagent Grade Water with 5 mL/L HOAc at 1 mL/minute	49
5.	Example Chromatogram of CGA-339833 and CGA-192155 Through a SB-CN Column Using 20% ACN:80% Reagent Grade Water with 5 mL/L HOAc and 0.75 g/L NH ₂ OAc at 1 mL/minute	50
6.	Example Chromatogram of a 0.020 µg/mL Standard for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	51
7.	Example Chromatogram of a 0.050 µg/mL Standard for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	52
8.	Example Chromatogram of a 0.20 µg/mL Standard for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	53
9.	Example Chromatogram of a 0.50 µg/mL Standard for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	54
10.	Example Chromatogram of a 1.0 µg/mL Standard for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	55

LIST OF TABLES AND FIGURES (con't)

Figures	Page
11. Example Chromatogram of a Method Blank Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column	56
12. Example Chromatogram of a Control Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	57
13. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	58
14. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	59
15. Example Chromatogram of a Control Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	60
16. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	61
17. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-339833 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	62
18. Example Chromatogram of a 0.020 µg/mL Standard for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	63
19. Example Chromatogram of a 0.050 µg/mL Standard for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	64
20. Example Chromatogram of a 0.20 µg/mL Standard for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	65
21. Example Chromatogram of a 0.50 µg/mL Standard for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	66
22. Example Chromatogram of a 1.0 µg/mL Standard for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	67

LIST OF TABLES AND FIGURES (con't)

Figures	Page
23. Example Chromatogram of a Method Blank Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column	68
24. Example Chromatogram of a Control Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	69
25. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	70
26. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (New Jersey Site)	71
27. Example Chromatogram of a Control Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	72
28. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	73
29. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-192155 Through a SB-CN Column and a Prodigy ODS2 Column (Georgia Site)	74
30. Example Chromatogram of a 0.020 µg/mL Standard for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column	75
31. Example Chromatogram of a 0.050 µg/mL Standard for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column	76
32. Example Chromatogram of a 0.20 µg/mL Standard for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column	77
33. Example Chromatogram of a 0.50 µg/mL Standard for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column	78
34. Example Chromatogram of a 1.0 µg/mL Standard for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column	79

LIST OF TABLES AND FIGURES (con't)

Figures	Page
35.1 Example Chromatogram of a Method Blank Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (New Jersey Site)	80
36.1 Example Chromatogram of a Control Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (New Jersey Site)	81
37. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (New Jersey Site)	82
38. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (New Jersey Site)	83
39. Example Chromatogram of a Control Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (Georgia Site)	84
40. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (Georgia Site)	85
41. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-265378 Through a SB-CN Column and a Zorbax ODS Column (Georgia Site)	86
42. Example Chromatogram of a 0.020 µg/mL Standard for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	87
43. Example Chromatogram of a 0.050 µg/mL Standard for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	88
44. Example Chromatogram of a 0.20 µg/mL Standard for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	89
45. Example Chromatogram of a 0.50 µg/mL Standard for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	90
46. Example Chromatogram of a 1.0 µg/mL Standard for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	91

LIST OF TABLES AND FIGURES (con't)

Figures	Page
47. Example Chromatogram of a Method Blank Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column	92
48. Example Chromatogram of a Control Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (New Jersey Site)	93
49. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (New Jersey Site)	94
50. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (New Jersey Site)	95
51. Example Chromatogram of a 1.0 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (New Jersey Site)	96
52. Example Chromatogram of a Control Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (Georgia Site)	97
53. Example Chromatogram of a 0.010 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (Georgia Site)	98
54. Example Chromatogram of a 0.10 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (Georgia Site)	99
55. Example Chromatogram of a 1.0 ppm Spiked Soil Extract for CGA-173506 Through a SB-CN Column and a Spherisorb ODS2 Column (Georgia Site)	100

I. INTRODUCTION/SUMMARY**A. Scope**

A method for the analytical determination of CGA-173506 and degradates (CGA-339833, CGA-192155, CGA-265378) in soil was developed by ABC Laboratories, Inc. (ABC), Columbia, MO. The limit of quantitation (LOQ) for all analytes is 0.010 µg/g (ppm) based on fortification experiments. The limit of detection (LOD) is 0.0025 µg/g (ppm) for CGA-339833 and CGA-192155 based on the lowest standard concentration injected with an 8 g/mL soil extract concentration. The LOD is 0.0050 µg/g (ppm) for CGA-265378 and CGA-173506 based on the lowest standard concentration injected with a 4 g/mL soil extract concentration. A two column switching HPLC system is used to quantitate samples with ultraviolet (UV) detection.

B. Principle

Extraction of analytes from the soil is accomplished by shaking for two, 10 minute periods with 90% acetonitrile (ACN):9% reagent grade water:1% glacial acetic acid (HOAc) containing 50 mg/L butylated hydroxy toluene (BHT). Solids are separated from the liquid extract by centrifugation. The extraction solvent is reduced to between 0.5 to 1 mL using vacuum rotary evaporation. The extract is then diluted to a 5 mL volume for injection onto the HPLC system for quantitation of CGA-265378 and CGA-173506. A 3 mL aliquot of the extract injected for CGA-265378 and CGA-173506 is then concentrated with a stream of nitrogen to a 1.5 mL volume prior to injection onto the HPLC system for quantitation of CGA-339833 and CGA-192155.

II. MATERIALS AND METHODS**A. Apparatus**

Similar apparatus may be used for this method if deemed acceptable.

- 1.0 Balance, analytical (Sartorius 1702 MP8) or equivalent
- 2.0 Balance, top loading (Mettler PM 200).
- 3.0 Bottle, polyethylene, Silgan disposable 8 oz round, wide mouth, disposable
- 4.0 Centrifuge, IEC Centra GP8
- 5.0 Centrifuge tubes, 15-mL graduated
- 6.0 Culture tubes, 16 X 125 mm glass
- 7.0 Cylinder, graduated 50-mL
- 8.0 Cylinder, graduated 1000-mL

- 9.0 Cylinder, graduated 2000-mL
- 10.0 Flasks, flat bottom, 500-mL
- 11.0 Funnels, powder, 75 mm
- 12.0 Glass wool (Fisher cat. # 11-388)
- 13.0 Pasteur pipets, disposable
- 14.0 Pipettes, glass, class A certified, various volumes
- 15.0 Pipettes, repeater pipettes, various volumes
- 16.0 Rotary evaporator, Strong Innovations
- 17.0 Syringe, Hamilton, 500 μ L
- 18.0 Vacuum pump (Welch 1402)
- 19.0 Ultrasonic bath (Branson 3200)
- 20.0 Vials, autosampler, clear, 12 X 32 mm, 2-mL
- 21.0 Vortex mixer (Thermolyne Maxi Mix II)

B. Reagents and Analytical Standards

Other brands of reagents may be substituted provided they are of equivalent purity, produce adequate recovery of all analytes, and a reagent blank produces no interferences. Use of other reagents has not been explored by ABC.

- 1.0 Acetic Acid, glacial, Fisher Scientific
- 2.0 Acetonitrile, HPLC grade, Burdick and Jackson
- 3.0 Ammonium Acetate, ACS reagent grade, Sigma
- 4.0 Butylated Hydroxy Toluene, Sigma
- 5.0 Dimethyl Sulfoxide, certified, Fisher Scientific
- 6.0 Reagent grade water (Type 1 water), Labconco Purification System
- 7.0 Phosphoric Acid, ACS reagent grade, J.T. Baker
- 8.0 CGA-339833, Standard reference material (Ciba-Geigy), Greensboro, NC
- 9.0 CGA-192155, Standard reference material (Ciba-Geigy), Greensboro, NC
- 10.0 CGA-265378, Standard reference material (Ciba-Geigy), Greensboro, NC
- 11.0 CGA-173506, Standard reference material (Ciba-Geigy), Greensboro, NC

C. Reagent Solutions and Mixtures

- 1.0 Extraction Solution: Combine 1800 mL of ACN with 100 ± 10 mg of BHT and mix to dissolve the BHT. After the BHT is dissolved, combine 180 mL reagent grade water and 20 mL of acetic acid (HOAc) with the ACN:BHT mixture and mix. Make fresh daily.
- 2.0 Dilution Solvent for Standards: Combine 100 mL of ACN, 395 mL of reagent grade water, and 5 mL of HOAc and mix.
- 3.0 Mobile Phase 1: Prepare 40% ACN:60% reagent grade water:5 mL/L HOAc (used for the isocratic chromatography of CGA-265378 and CGA-173506 on the first column; a Zorbax SB-CN HPLC column). For each liter of mobile phase, combine 400 mL of ACN with 600 mL of reagent grade water and add 5 mL/L HOAc. Mix the solution by stirring. Filter through a 0.45 µm filter membrane using a vacuum or sparge with helium for a minimum of 30 minutes before use.
- 4.0 Mobile Phase 2: Prepare 20% ACN:80% reagent grade water:5 mL/L HOAc:0.1 to 1.5 g/L NH₄OAc (used for the isocratic chromatography of CGA-339833 and CGA-192155 on the first column, a Zorbax SB-CN HPLC column). For each liter of mobile phase, combine 200 mL of ACN with 800 mL of reagent grade water, add 5 mL/L of HOAc and an amount of NH₄OAc that will give separation of CGA-339833 and CGA-192155 with a minimum of a 5 mL retention volume for the CGA-339833 peak. Mix the solution by stirring. Filter through a 0.45 µm filter membrane using a vacuum or sparge with helium for a minimum of 30 minutes before use.
- 5.0 Mobile Phase 3: Prepare 90% ACN:10% reagent grade water:5 mL/L HOAc (used to regenerate the first column, a Zorbax SB-CN HPLC column). For each liter of mobile phase, combine 900 mL of ACN with 100 mL of reagent grade water and add 5 mL/L of HOAc. Mix the solution by stirring. Filter through a 0.45 µm filter membrane using a vacuum or sparge with helium for a minimum of 30 minutes before use.
- 6.0 Mobile Phase 4: Prepare 40% ACN:60% reagent grade water:5 mL/L HOAc:0.20 g/L NH₄OAc (used isocratically on the second columns, which are Prodigy ODS2 for the determination of CGA-339833 and CGA-192155). For each liter of mobile phase, combine 400 mL of ACN with 600 mL of reagent grade water. Add 5 mL of HOAc and 0.20 g NH₄OAc for each liter of mobile phase. Mix the solution by stirring. Filter through

a 0.45 μm filter membrane using a vacuum or sparge with helium for a minimum of 30 minutes before use.

- 7.0 Mobile Phase 5. Prepare 50% ACN:50% reagent grade water:5 mL/L HOAc (used isocratically on the second columns, a Zorbax ODS and Spherisorb ODS2 HPLC columns for the determination of CGA-256378 and CGA-173506, respectively). For each liter of mobile phase, combine 500 mL of ACN with 500 mL of reagent grade water and add 5 mL/L of HOAc for each liter of mobile phase. Mix the solution by stirring. Filter through a 0.45 μm filter membrane using a vacuum or sparge with helium for a minimum of 30 minutes before use.

D. **HPLC Columns and Supplies**

Substitution of HPLC column brands may be acceptable if similar retention characteristics and freedom from matrix interferences can be demonstrated. If other columns are substituted, the secondary separation characteristics (ammonium ion concentration) for the substituted columns will have to be explored. The secondary interactions related to the SB-CN column are strong for all the analytes, while secondary interactions for CGA-339833 and CGA-192155 are also very strong on the ODS columns used. See the section, K.1.0, Discussion of Special Chromatographic Separations Achievable, for help regarding HPLC column selection.

- 1.0 4.6 X 150 mm ZorbaxTM SB-CN (5 μm) column (cat no. 883975.905)
- 2.0 4 X 12.5 mm Zorbax SB-CN (5 μm) cartridge guard column (cat no. 820674.916)
- 3.0 Zorbax RelianceTM guard column hardware kit (cat no. 820529.901)
- 4.0 4.6 X 250 mm Zorbax ODS (5 μm) column (cat no. 880952.702)
- 5.0 4.6 X 250 mm Phenomenex ProdigyTM 5 ODS2 (5 μm) column (cat no. 006-3300-E0)
- 6.0 4.6 X 250 mm SpherisorbTM ODS2 (5 μm) cartridge column (Phase Separations part no. 839540)
- 7.0 Column end fittings for Spherisorb cartridge columns (Phase Separations part no. 614100)

E. Safety and Health

As the reference substances used in this analysis have not been completely evaluated at this time, general laboratory safety is advised (e.g., safety glasses, gloves, etc. should be used).

F. Standard Solutions

After preparation, standard solutions are to be stored in brown glass bottles. Structures for each of the four analytes are presented in Figure 1.

1.0 Primary Stock Standard Solutions. Each primary stock standard solution is prepared individually by weighing the respective reference material into a weigh boat to achieve an approximate 10 mg weight. The weight of the individual reference material is recorded (to 0.1 mg), and the material is transferred to a 50 mL volumetric flask using 10 mL of ACN. The standard for CGA-173506 is diluted with ACN to volume.

The remaining standard solutions have 30 to 35 mL reagent grade water added to each; then 0.5 mL HOAc added to the volumetric, and the volumetric swirled to mix the contents. The solution is then made to volume with reagent grade water. The solutions are again mixed by inversion or, an ultrasonic bath may be used to assure the reference materials are in solution. The concentration of each stock standard solution, corrected for percent purity, is calculated. Primary stock solutions are to be stored in a freezer (approximately -20 °C) when not in use.

2.0 Stock Mixed Standard and Spiking Solutions. Mixed standard and spiking solutions are made by diluting the primary stock standards using dilution solvent (20% ACN:79% reagent grade water:1% HOAc). The stock mixed standard is prepared by adding an aliquot of the individual stock standard solution containing 1000 µg of the reference standard to a 100-mL volumetric flask. The 100-mL flask is then diluted to volume with dilution solvent to give a 10 µg/mL mixed standard solution. The 10 µg/mL mixed standard solution is also diluted to make a 1 µg/mL mixed standard spiking solution. All mixed standard solutions should be stored refrigerated (approximately 4 °C) when not in use. Make fresh every three months.

3.0 Standard Curve Solutions. The standard curve, used to calibrate the instrument, is prepared by dilution of the 10 µg/mL mixed standard. Standards are prepared by dilution with standard diluent to be 1.0, 0.50,

0.20, 0.050, and 0.020 $\mu\text{g}/\text{mL}$. All mixed standard solutions should be stored refrigerated (approximately 4 °C) when not in use. Make fresh monthly.

The 0.020 $\mu\text{g}/\text{mL}$ concentration should be used in the standard curve for the determination of CGA-265378 and CGA-173506. The 0.020 $\mu\text{g}/\text{mL}$ standard level may be omitted from the standard curve for CGA-339833 and CGA-192155 determinations as the matrix concentration for these analytes is double that of the CGA-265378 and CGA-173506 screening levels. The different standard concentrations are injected onto the chromatograph to bracket and develop a standard response curve for a defined group of samples. The standard curve solutions are also used to spike fortified samples.

- 4.0 Individual Analyte Spiking and Standard Curve Solutions. Individual standard solutions are prepared by pipetting an aliquot of primary standard solution, equivalent to 400 μg , into a 100-mL volumetric flask and diluting with dilution solvent. This 4 $\mu\text{g}/\text{mL}$ standard is then serially diluted to give an individual HPLC injection standard by diluting 10 mL of the 4 $\mu\text{g}/\text{mL}$ standard solution to 50 mL with dilution solvent. This 0.80 $\mu\text{g}/\text{mL}$ standard solution may be used to identify retention times for the individual analytes.

G. Sample Extraction

Step by step instructions follow for extraction of soil and preparation of the concentrated extract for injection onto an HPLC system. Figure 2 gives the steps for extract production in a flow chart format.

- 1.0 Weigh 20 ± 0.1 g of soil into a 250-mL plastic bottle.
- 2.0 Fortification solutions are added at this time to fortify samples at the appropriate level. Allow the fortification solutions to remain on the matrix for 5 to 10 minutes prior to addition of extraction solvent.
- 3.0 Add 100 mL of extraction solvent (90% ACN:9% reagent grade water:1% HOAc + 50 mg/L BHT) to each sub sample contained in a 250 mL bottle. Cap the bottles and place on a linear oscillating shaker for 10 minutes on high (280 oscillations/minute).
- 4.0 Remove the bottles from the shaker and place into groups of two. Balance each pair of bottles by adding extraction solvent to have the gross weight

• Pairs of extraction bottles agree to within 0.1 g. Place each group across from each other on the centrifuge.

5.0 Centrifuge at 3000 rpm for 2 minutes or a longer period as required to produce a clear supernatant.

6.0 Remove the bottles from the centrifuge. Decant the extraction liquid through a powder funnel plugged with glass wool (to remove the floating particulate matter) fitted on top of a 500-mL flat bottom flask.

7.0 Add 50 mL of extraction solvent and resuspend the solids by capping the extraction bottle and shaking by hand vigorously. Then place the bottles on the shaker on high for a second, 10 minute shaking period.

8.0 Again, balance the pairs of extraction bottles with extraction solvent as indicated in step 4 above and centrifuge as in step 5 above.

9.0 The liquid is decanted through the same glass wool plug as the initial extraction solvent into the same 500-mL flat bottom.

10.0 The glass wool plug is rinsed with 10 mL of extraction solvent and the glass wool plug is discarded.

11.0 The volume of the extract is reduced to 0.5 to 1 mL by vacuum rotary evaporation using a 20 to 40 °C water bath. By starting out the evaporation in a colder water bath, foaming and bumping may be avoided. After most of the ACN has been evaporated, drain the evaporation traps, and warm the water bath to speed the evaporation of the aqueous portion of the extract.

Note that in order to achieve acceptable recoveries, steps 12 to 15 must be followed!

12.0 Transfer the remaining extract volume to a 15-mL graduated centrifuge tube. Pipet 2.0 mL of ACN into the 500-mL flat bottom flask.

13.0 Grasp the neck of the flask and hold the flask so that the neck is in a horizontal position. While in this position, turn and swirl the flask in an ultrasonic bath so that the solids on the sides of the flask come into contact with the ACN while in the ultrasonic bath. The flask should be rotated a minimum of three revolutions over a 30 second period while holding the flask in a horizontal position, in order to dislodge the solids deposited in a

ring during rotary evaporation. The flask is then turned so that the flat bottom portion of the flask rests on the bottom of the ultrasonic bath, and the ACN and solids contained in the flask are sonicated for another 15 seconds.

The ACN rinse from the flat bottom flask is then transferred to the 15-mL centrifuge tube containing the original extract. Two milliliters of reagent grade water is then added to the flat bottom flask and the sonication process in the paragraph above is repeated.

The aqueous rinse from the flat bottom flask is added to the 15-mL centrifuge tube. If the volume of the tube goes above 5.0 mL, reduce the volume with a stream of nitrogen and a 30 to 40 °C water bath to achieve a 5.0 mL volume. If the volume of the tube is below 5.0 mL, add reagent grade water to achieve a 5.0 mL volume. Vortex the 15-mL centrifuge tube briefly and centrifuge for 10 minutes on a table top centrifuge.

- 13.0 Transfer 3.0 mL of the extract from step 12 above to a fresh 15-mL centrifuge tube using care not to disturb the solids. Use a stream of nitrogen and a 30 to 40 °C water bath to reduce the volume of the extract to 1 to 1.5 mL. Bring the volume of the extract to 1.5 mL with reagent grade water, vortex, and centrifuge for 10 minutes on a table top centrifuge. Place the extract into an injection vial and analyze for CGA-339833 and CGA-192155.
- 14.0 Transfer an aliquot of the solution from step 12 above to an injection vial. Use care to avoid transfer of solids and analyze for CGA-265378 and CGA-173506.
- 15.0 If sample extract dilutions are required for analyte response to be within the analytical curve, then dilute with dilution solvent used for the standards (20 ACN:79 reagent grade water:1 HOAc).

K.3.3.1 HPLC Chromatography (General Discussion)

A Shimadzu HPLC system was used to chromatograph the extracts and standards for this method. Similar instruments are acceptable substitutes. The system used employs three analytical HPLC columns with column to column switching and UV detection. A schematic of the hydraulic configuration for the analytical system is shown in Figure 3. General instrument parameters are given below.

Adjustment of mobile phase conditions may be required to provide resolution from matrix peaks and produce desirable retention times. In general, mobile phases must produce retention times providing 4 to 10 column void volumes. The retention volume for the first analyte peak on the first column should be 3 to 5 column volumes. The last analyte peak should apex at no more than 12 column volumes for the first column. All columns used as the second column should provide 4 to 8 column volumes. If the columns specified do not provide these retention volumes, then the mobile phases should be adjusted. See the section, K.1.0, Discussion of Special Chromatographic Separations Achievable in this report to afford easier mobile phase component adjustments.

Individual instrument parameters are included with each analytical run. Conditions may vary from the general description given below to account for variations in mobile phase preparation and the retention time variation of individual columns.

1.0 Injection Volume. Inject 200 μ L for CGA-265378 and CGA-173506 or 300 μ L for CGA-339833 and CGA-192155. If adequate signal to noise is achieved for the lowest standard, lower injection volumes may be used.

2.0 Autosampler Rinse Solution. 40% ACN:60% reagent grade water.

3.0 UV Detection.

Compound	Wavelength
CGA-339833	275 nm
CGA-192155	285 nm
CGA-265378	268 nm
CGA-173506	268 nm

I. HPLC Analysis of CGA-265378 and CGA-173506 (non-polar analytes)**1.0 First Column Specifications**

A Zorbax SB-CN 4.6 mm internal diameter by 15 cm length with 5μ CN packing material with a Zorbax SB-CN 4 X 12.5 mm cartridge guard column was used as the first column. A similar column may be used if analyte and matrix peaks are demonstrated to be resolved adequately. Since this is the initial column used, recovery of analytes and separation of matrix coextractive peaks through both columns must be demonstrated.

2.0 First Pump Flow Rate

A flow rate of 0.7 to 1.5-mL/min may be used for this analysis. The normal flow rate is 1.0 mL/min, but may be lowered or raised depending on the back pressure of the analytical columns during the column switching time when the two columns are connected in series.

3.0 First Column Mobile Phase for CGA-265378 and CGA-173506

A 40% ACN:60% reagent grade water with 5 mL/L HOAc (Mobile Phase 1) is used to elute the analytes isocratically from the first column. After the analytes have eluted from the first column, the mobile phase is immediately taken to 90% ACN:10% reagent grade water with 5 mL/L HOAc at 2 mL/min (Mobile Phase 3) for 5 minutes to remove the strongly retained soil coextracted compounds. After 5 minutes of pumping mobile phase 3, mobile phase 1 is again pumped for 10 minutes at 2 mL/min to equilibrate the column prior to the next injection. The 2 mL/min flow rate is lowered to 1 mL/min for at least 1 minute prior to the next injection to allow for flow rate consistency during the next injection.

4.0 Normal Retention Times for Column 1 at 1 mL/min flow

Compound	Time (min)
CGA-265378	7 - 8
CGA-173506	9 - 11

An example chromatogram for the two analytes with the mobile phase and conditions specified above is shown as Figure 4. The peaks in this chromatogram for CGA-192155 and CGA-339833 are shown to demonstrate their elution order relative to the non-polar compounds. Variations in columns or mobile phase can cause these two compounds to

move such that they may co-elute. They will be separated from the non-polar compounds on the ODS2 columns.

5.0 Establishment of Switching Valve Times

The SB-CN column is eluted with 1.0 mL/min of mobile phase 1. The eluant from the column is directed to a UV detector set at 268 nm wavelength. Chromatograms are acquired for three replicate injections of the 1.0 $\mu\text{g}/\text{mL}$ standard. Retention times for each of the analytes must be within 0.1 minutes for each of the three injections. If retention times are not within ± 0.05 minutes, the system should be evaluated and/or repaired before analysis is started. The column should be timed for the volume of injection to be used for analysis. Different injection volumes will influence the retention times. To correctly set the peak window, the same injection volume must be used for timing as used for the analysis.

The peak tailing factor (calculated at 5% of peak height)³ should be less than 1.8 for all of the analytes eluting from the SB-CN column. If excessive tailing is observed, replacement of the guard column is indicated. If peak tailing is still unsatisfactory, replacement of the analytical column is indicated.

Establishment of switching valve times for the SB-CN column should be performed routinely after any of the following have occurred; 1) The column has not been used for a day, 2) A new mobile phase is made, 3) Any suggestion of retention time shifting such as drifting peak height response after the second column, or 4) Injection volume is changed.

Switching valve times for transfer of the eluant from the first column to the second column are set so that the transfer times will encompass all three injections made during the column timing procedure. This is accomplished by overlaying chromatograms acquired during column timing. The switching valve initiation time is set to be just as the analytical peak rises from the base line. The switching valve return time is set to be just as the peak tail comes back to base line.

The switching valves are placed in series (see Figure 3) so that the flow from the SB-CN column can enter the first valve (Valve A) and can be directed to a second column. When Valve A is in the initial position, the flow continues through Valve A and into Valve B. As either valve position is changed, the flow from the SB-CN column is directed onto the second column.

6.0 Second Columns

Two, 4.6 mm internal diameter x 25 cm length ODS ($5\mu\text{m}$), columns are used as the second column for the analysis of both CGA-265378 and CGA-173506. The two columns are used by connecting each one of the columns to a switching valve (see Figure 3). A Spherisorb ODS2 cartridge column (CGA-173506 cut) or a Zorbax ODS column (CGA-265378 cut) have both been used successfully as second columns to chromatograph these extracts for the respective compounds.

7.0 Pump Flow Rates for Second Columns

A flow rate of 1 to 2-mL/min may be used for these columns. The normal flow rate is 1.0 mL/min, but may be lowered or raised depending on the back pressure of the analytical column.

8.0 Second Column Mobile Phase

The mobile phase used for both columns is 50% ACN:50% reagent grade water with 5 mL/L HOAc (Mobile phase 5).

J. HPLC Analysis of CGA-339833 and CGA-192155 (polar analytes)**1.0 First Column**

Specifications of the first column are the same as that column listed under section I.1.0. A similar column may be used if analyte and matrix peaks are demonstrated to be resolved adequately. Since this is the initial column used, recovery of analytes and freedom from matrix coextractive peaks through both columns must also be demonstrated.

2.0 First Pump Flow Rate

A flow rate of 0.7 to 1.5-mL/min may be used for this analysis. The normal flow rate is 1.0 mL/min, but may be lowered or raised depending on the back pressure of the analytical columns during the column switching time when two columns are connected in series.

3.0 First Column Mobile Phase for CGA-339833 and CGA-192155

A 20% ACN:80% reagent grade water with 5 mL/L HOAc and 0.1 to 1.5 g/L NH₄OAc (Mobile Phase 2) is used to elute the analytes isocratically from the first column. After the analytes have eluted from the first

column, the mobile phase is immediately taken to 90% ACN:10% reagent grade water with 5 mL/L HOAc at 2 mL/min (Mobile Phase 3) for 5 minutes to remove the strongly retained soil coextracted compounds. After 45 minutes of pumping mobile phase 3, mobile phase 2 is again pumped for 10 minutes at 2 mL/min to equilibrate the column prior to the next injection. The 2 mL/min flow rate is lowered to 1 mL/min for at least 1 minute prior to the next injection to allow for flow rate consistency during the next injection.

4.0 Normal Retention Times for Column 1 at 1 mL/min flow

Compound	Time (min)
CGA-339833	7 - 8
CGA-192155	9 - 11

An example chromatogram for the two analytes with the mobile phase and conditions specified above is shown as Figure 5.

5.0 Establishment of Switching Valve Times

The SB-CN column is eluted with 1.0 mL/min of mobile phase 2 and the eluant from the column directed to the UV detector set at 268 nm wavelength. Chromatograms are acquired for three replicate injections of the 1.0 μ g/mL standard. Retention times for each of the analytes must be within 0.1 minutes for each of the three injections. If retention times are not within \pm 0.05 minutes, the system should be evaluated and/or repaired before analysis is started. The column should be timed for the volume of injection to be used for analysis. Different injection volumes will influence the retention times, and the peak window may be set incorrectly.

The peak tailing factor (calculated at 5% of peak height)¹ should be less than 1.8 for all of the analytes eluting from the SB-CN column. If excessive tailing is observed, replacement of the guard column is indicated. If peak tailing is still unsatisfactory, replacement of the analytical column is indicated.

Establishment of switching valve times for the SB-CN column should be performed routinely after any of the following have occurred; 1) The column has not been used for a day, 2) A new mobile phase is made, 3) Any suggestion of retention time shifting such as drifting peak height response after the second column, or 4) Injection volume is changed.

Switching valve times for transfer of the eluant from the first column to the second columns are set so that the transfer times will encompass all three injections made during the column timing procedure. This is accomplished by overlaying chromatograms acquired during column timing. The switching valve initiation time is set to be just as the analytical peak rises from the base line. The switching valve return time is set to be just as the peak tail comes back to base line.

The switching valves are placed in series (see Figure 3) so that the flow from the SB-CN column can enter the first valve (Valve A) and can be directed to a second column. When Valve A is in the initial position, the flow continues through Valve A and into Valve B. As either valve position is changed, the flow, from the SB-CN column is directed onto the second column.

6.0 Second Columns

Two, 4.6 mm internal diameter x 25 cm length (5 μ m) Prodigy ODS2, columns are used as the second column for the analysis of both CGA-339833 and CGA-192155. The two identical columns are used by connecting each one of the columns to a switching valve (see Figure 3). Best results have been obtained by using the specified ODS2 columns.

7.0 Pump Flow Rates

A flow rate of 1 to 2 mL/min may be used for these columns. The normal flow rate is 1.0 mL/min, but may be lowered or raised depending on the back pressure of the analytical column.

8.0 Second Column Mobile Phase

The mobile phase used for both columns is 40% ACN:60% reagent grade water with 5 mL/L HOAc and 0.2 g/L NH₄OAc (Mobile phase 4).

K. Modifications and Potential Problems

1.0 Discussion of Special Chromatographic Separations Achievable

All of these special conditions are discussed to enable the chromatographer to prepare mobile phases that may be used to resolve analytes from matrix peaks if needed. Additionally, when starting with new columns, the chromatographer may not be able to use the same mobile phases indicated in this method for the SB-CN or the Prodigy ODS2 columns. Hopefully, this discussion will be a valuable aid in establishing acceptable chromatography conditions with new columns, or provide an analyst unfamiliar with this method some insight into the special separation characteristics related to the SB-CN and the Prodigy ODS2 columns.

Chromatographic separation and retention times are dependent on ACN concentration for all analytes on all columns and all compounds do respond in a reverse phase manner. Additionally, separation and retention time for CGA-339833 and CGA-192155 rely heavily on ammonium ion concentration (0 to 2 g/L NH₄OAc) on both the Zorbax SB-CN column and the Prodigy ODS2 under acidic conditions (5 mL/L HOAc). CGA-339833 and CGA-192155 retention times on both columns decrease as the ammonium ion concentration increases with the acidity and ACN levels held constant. The retention time effect of ammonium ion concentration is greater for CGA-339833 on both the Prodigy ODS2 and the SB-CN column than for CGA-192155. The difference in ammonium ion effect for CGA-339833 and CGA-192155 on both these columns (SB-CN and the Prodigy ODS2) is so great that the elution order of CGA-339833 and CGA-192155 can be inverted. Additionally, CGA-339833 may not elute from these columns in the absence of ammonium ion. It has been found that all of these conditions identified for individual columns are able to provide stable retention times for analysis.

2.0 Separations on the SB-CN Column

To find the proper concentration of ammonium ion, it is easier to prepare a 20% ACN:80% reagent grade water mobile phase with 5 mL/L HOAc, remove a portion of that mobile phase and add enough NH₄OAc to attain a 2 g/L concentration. By using the gradient pumps to mix these mobile phases, one can quickly identify the proper concentration of NH₄OAc to achieve acceptable retention and resolution for CGA-339833 and CGA-192155 on the SB-CN column.

By using different concentrations of NH₄OAc, the retention times for CGA-339833 will move greatly, while CGA-192155 will move to a lesser extent. Separation of the CGA-339833 and CGA-192155 from each other, or from matrix interferences may be achieved by adjusting the NH₄OAc and ACN concentrations in the mobile phase.

Retention times for CGA-265378 and CGA-173506 are not affected by NH₄OAc. When using the 20% ACN mobile phase discussed in this section, the retention times for both the CGA-265378 and CGA-173506 analytes is greater than 20 column volumes, however, if the mixed standards are used to time the columns, these compounds will eventually elute.

3.0 Separations on ODS Columns

Evaluation of ammonium ion concentration on ODS columns gave a more pronounced effect for CGA-339833 than for CGA-192155. An ammonium ion effect was not noted for CGA-265378 and CGA-173506. It has been found that the use of the Prodigy ODS2 column does not provide the resolution for matrix peaks for both CGA-265378 and CGA-173506 that the Zorbax ODS and Spherisorb ODS2 columns provide, respectively.

All of these ammonium ion interactions, in combination with ACN concentration on both the SB-CN and the ODS columns, may be used to enhance resolution from matrix peaks (interferences) if the need arises.

4.0 Regeneration of SB-CN HPLC Columns

After extended use of the SB-CN column, it has been found that the peak shape deteriorates. This is evidenced by tailing or split peaks found during timing of the SB-CN column. These columns have been successfully restored to obtain the original peak shapes for all analytes by pumping 40 to 60 mL of 100% dimethyl sulfoxide through the column with the flow reversed through the column.

5.0 Loss of Analytes

Recovery of analytes can be influenced by the technique used when reconstituting the rotary evaporated soil extract. It is imperative that the reconstitution method be followed as indicated in this method and the soil extracts be used and generated as indicated in this method.

The polar metabolites (CGA-173506 and CGA-265378) partition into the soil coextracted material and must be removed by the addition of ACN first, then sonication used to remove the analytes from the precipitated soil extracts. This ACN rinse is then transferred from the flask, and finally the flask rinsed with reagent grade water.

The concentrated extracts injected for the polar metabolites (CGA-339833 and CGA-192155), should not be used for the analysis of the non-polar metabolites. The non-polar metabolites partition into the precipitated soil coextractives generated by removing the ACN during concentration.

The non-polar metabolite extracts should not be used for analysis of the polar metabolites as the level of ACN will cause the polar metabolites to move from the retention window established for column switching on the first column.

During development of this method, it was noted that CGA-265378 recoveries were severely reduced in the presence of acetone or ethyl ether. It was hypothesized that there was an oxidative conversion to some other unidentified analyte. Low recoveries were also noticed with increased soil organic matter such as found in the thatch-sod (0 to 7.5 cm) from a turf plot study. In order to potentially buffer this loss, the initial method contained 50 ppm BHT in the extraction solution.

6.0 Confirmatory Techniques

No confirmatory analysis procedure has been developed at this time.

7.0 Time Requirement
A set of 12 samples can be extracted during a six hour period by one person.

Chromatography is accomplished using automated equipment. A set of twelve samples will require 20 injections of extracts and standards at a run time of about 30 minutes each. An entire set of extracts can be injected in about 10 hours. Data reduction requires an additional 2 hours.

Injection of the set must be repeated in order to acquire data for the second group of analytes. The same amount of time will be required for the

second injection set. The total instrument time required for a set of 12 samples is approximately 20 hours.

L. Data Acquisition and Calculations

MULTICHROM™ is a computer program in use at ABC which allows for data acquisition, data analysis, results reporting, and information management. Peak response for standards and sample extracts are measured using the MULTICHROM system. The MULTICHROM system uses the concentration ($\mu\text{g/mL}$) versus peak response to form a regression curve and from that interpolate the concentration of analytes in the extracts. This value is then converted to parts per million (ppm) in the sample by entering the final sample volume, any dilution factors, and the initial sample weight into the MULTICHROM program. MULTICHROM calculates sample concentrations according to the following equation:

$$\text{ppm found} = \frac{(\mu\text{g/mL found}) \times (\text{final volume mL}) \times (\text{dilution factor})}{\text{sample weight (g)}}$$

The dilution factor if required, is calculated as follows. If no dilution is needed, then a 1 is entered into the calculation.

$$\text{dilution factor} = \frac{\text{final volume (mL)}}{\text{aliquot volume (mL)}}$$

Data from the MULTICHROM program are then entered into Excel® to calculate the recovery of fortified samples. Recovery of the fortified samples is calculated by subtracting the peak response for the control (average if more than one control is in a sample set) from the peak response of the fortified samples and then interpolating the concentration in the fortified extract. Recovery is then calculated according to the following formula:

$$\text{percent recovery} = \frac{(\text{ppm found} \times 100)}{\text{ppm fortified}}$$

Moisture determinations for samples are performed according to the ABC soil moisture determination SOP FC 1.7.3. This SOP requires that samples be dried in an oven at 105 °C overnight, removed and weighed. Samples are returned to the oven for a second drying period and reweighed to prove that the second dry weight is within 1% of the first dry weight. If the first dry weight and the second dry weight do not agree, then the SOP provides for a third drying period with the

SL to the soil moisture and weight of the soil sample. The expected 1% agreement still in effect. The actual calculation for soil moisture is defined by the formula with all weights recorded in grams:

$$\text{soil moisture \%} = \frac{[(\text{Wet sample} + \text{container wt}) - (\text{Dry sample} + \text{container wt})] \times 100}{(\text{Wet sample} + \text{container wt}) - (\text{weight of container})}$$

Sample moisture is then used to correct sample residue levels for moisture content on a dry weight basis. The formula used to correct for moisture content is given by:

$$\text{ppm corrected} = \frac{\text{ppm found} \times 100}{100 - \text{soil moisture \%}}$$

Method No. CGA011696/Soil Revision No. 05 Page 26

(4) Calculations

Method No. CGA011696/Soil Revision No. 05 Page 26

(5) Results

Method No. CGA011696/Soil Revision No. 05 Page 26

III. RESULTS AND DISCUSSION

This method was validated under Study/Protocol numbers Ciba 32-95² and Ciba 33-95³. The ABC study numbers were 42162 and 42163. The objective of these protocols was to conduct a soil dissipation study for CGA-173506 and degradates. Part B of these protocols outlined the analytical methods, method validation, analysis of samples, and a storage stability study for the analytes. Table I gives soil characterization data for both studies.

Data derived from the chromatography of standards and extracts for the New Jersey site method validation (Ciba No. 32-95 and ABC No. 42162) are presented in Table II for each analyte. Data for the chromatography of standards and extracts from the Georgia site method validation (Ciba No. 33-95 and ABC No. 42163) are presented in Table III for each analyte.

Table IV gives summary data for each of the analytes. Recovery for each level is indicated as well as the average recovery, standard deviation, relative standard deviation (RSD), and recovery range.

Figure 1 gives the molecular structure for each of the analytes. Figure 2 provides the extraction and analysis scheme in a flow chart. Figure 3 provides the hydraulic configurations of the HPLC equipment used to conduct these analyses.

Figures 6 to 55 provide example chromatograms for standards, extracts from reagent blanks, control soil, and fortified control soil from Georgia and New Jersey soil dissipation study sites. Chromatograms are shown for each analyte.

Currently, ABC is conducting soil dissipation studies using this method on the soils sampled from the two sites used to validate this method. While analyzing samples taken from those sites, 10 to 20% of the total samples are fortified samples. Although this data is not reported in this method, it has been found that this method meets the required 70 to 120% average recovery and less than 20% RSD for CGA-173506, CGA-192155, and CGA-339833. The RSD for CGA-265378 to date has exceeded 20%.

IV. CONCLUSIONS

The method, as validated, provides an adequate means of analysis for the four analytes given (as indicated in summary Table IV). The average recovery ranged from 83 to 107% for all fortification ranges and analytes. The standard deviation ranged from 3.4 to 20% for all fortification ranges and analytes.

The method has been established for the analysis of soil samples. The method is capable of determining the four analytes at the specified detection limits.

It is recommended that the method be used to determine the analytes in soil samples.

The method has been established for the analysis of soil samples. The method is capable of determining the four analytes at the specified detection limits.

The method has been established for the analysis of soil samples. The method is capable of determining the four analytes at the specified detection limits.

The method has been established for the analysis of soil samples. The method is capable of determining the four analytes at the specified detection limits.

V. CERTIFICATION


This method and experimental results are certified to be authentic accounts of the method validation data contained in ABC study numbers 42162 and 42163 (Ciba study numbers 32-95 and 33-95). Original raw data is currently at ABC and will remain there until the soil dissipation studies are finalized. After the studies are finalized, a copy of the raw data will remain at ABC and the original raw data will be archived by Ciba-Geigy.

Soil from the validated sites is currently being stored at ABC. After finalization, soil will be transferred to Ciba-Geigy at the study directors request.

Reference standard materials were characterized and supplied by Ciba-Geigy. Ciba-Geigy will maintain a supply of standard reference materials.

5 Nov 96

Date




Michael E. Gresham
Analytical Study Coordinator
Analytical Chemistry and Field Studies
Group
ABC Laboratories, Inc.

VI. CERTIFICATION OF GOOD LABORATORY PRACTICES


The analytical work reported in ABC Method No. CGA011696/Soil was performed as a part of study numbers 42162 and 42163 (Ciba study numbers 32-95 and 33-95). These studies are being conducted in accordance with Good Laboratory Practice Standards, 40 CFR Part 160.

05 Nov 96
Date





Michael E. Gresham
Analytical Study Coordinator
Analytical Chemistry and Field Studies Group
ABC Laboratories, Inc.

11/7/96
Date



Thomas Wiepke, Ph.D.
Study Director
Environmental Fate & Effects Department
Ciba-Geigy Corporation
Greensboro, NC 27419-8300

11/11/96
Date


Robert K. Williams 
Manager
Environmental Residue Studies
Environmental Fate & Effects Department
Ciba-Geigy Corporation
Greensboro, NC 27419-8300

VII. QUALITY ASSURANCE STATEMENT

The analytical work reported in ABC Method No. CGA011696/Soil was inspected and/or audited as a part of study numbers 42162 and 42163 (Ciba study numbers 32-95 and 33-95). The findings pertinent to the data reported herein have been reported to the Analytical Study Coordinator, ABC Management, and the Study Director on the dates listed below.

Inspection/Audit Type	Inspection/Audit Date (s)	Reporting Date (Study Director)
Protocol (ABC No. 42162)	01-23-96	01-26-96
Protocol (42162 and 42163)	03-06-96	03-15-96
Extraction (42162 and 42163)	3-14-96	03-25-96
Draft Method	08-13-96	08-20-96
Final Method	08-13-96	08-20-96
Final Method	11-05-96	11-07-96

11-5-96

Date

Casey Howell

Casey Howell
Quality Assurance Specialist
Analytical Chemistry and Field Studies
Group
ABC Laboratories, Inc.

Table I Soil Characterization Data

Soil Depth	0-6" (0-15 cm)	0-6" (0-15 cm)
pH	6.8	7.3
Cation Exchange Capacity (meq/100 g)	9.8	4.7
% Organic Matter	2.0	0.9
% Water Holding Capacity @ 1/3 Bar	22.9	5.2
% Sand	28	88
% Silt	52	7
% Clay	20	5
Soil Classification	Silt Loam	Sand
Bulk Density (g/cc)	1.09	1.47

Soil Characterization Performed by Agvise Laboratories, Northwood, ND

Table II (cont.) Calibration and Recovery Data for New Jersey Soil

Time	Plot	Soil	Rep.	Lab	PPM	Sample	Sample	Sample	Dil.	PPM	Recovery	Percent
Point	Site	Depth	Ab	No.	Spike	Extract	Analysis	Number	Date	Pac.	Hei	Recovery
TIB-NJ-TR	00-06-A-B & C	1.2-con	3	3/25/96	03/23/96	3	0.5	3237.2	0.0037	112		
TIB-NJ-TR	00-06-A-B & C	2.2-con	3	3/25/96	03/23/96	4	0.5	7845.5	0.0060	14		
TIB-NJ-TR	00-06-A-B & C	3.2-con	3	3/25/96	03/23/96	5	0.5	17670.1	0.0096	19		
TIB-NJ-TR	00-06-A-B & C	4.2-con	3	3/25/96	03/23/96	6	0.5	31502.1	0.0069	16		
TIB-NJ-TR	00-06-A-B & C	5.2-con	3	3/25/96	03/23/96	8	0.5	34927.1	0.0059	17		
TIB-NJ-TR	00-06-A-B & C	6.2-con	3	3/25/96	03/23/96	9	0.5	19218.1	0.0052	15		
TIB-NJ-TR	00-06-A-B & C	7.2-con	3	3/25/96	03/23/96	10	0.5	106143.1	0.0971	971		
TIB-NJ-TR	00-06-A-B & C	8.2-con	3	3/25/96	03/25/96	11	0.5	112089.1	0.1030	103		
TIB-NJ-TR	00-06-A-B & C	9.2-con	3	3/25/96	03/25/96	13	0.5	611.1	0.0000	41		
TIB-NJ-TR	00-06-A-B & C	10.2-con	3	3/25/96	03/25/96	14	0.5	526.1	0.0000	0		
Reagent Blank						11.2	15	0.5	222.19	0.0000	79	
0.80 ug/mL CGA-192155 ONLY						15	16	1:115309	0.8493	J06		
0.80 ug/mL CGA-339833 ONLY						17	17	13 ^a	0.0000	0		
						17	17	13 ^a	0.0000	0		
						17	17	13 ^a	0.0000	0		

Sample #s 9, 2 and 10, 2 are fortified with CGA-173506 only. They are calculated for % conversion for the other compounds. Final Vol. = 5 mL Sam. Wt. = 20g MC Ch. #15 File: MV3 pg/mL Comp.: CGA-192155

127849 0.9995
 0.3/25/96 2 0.5 63968 0.4940 r = 0.99975
 0.3/25/96 7 0.2 27578 0.2060 m = 126365
 0.3/25/96 12 0.2 28512 0.2134 b = 1346

^a Average control response (6441)
 is subtracted prior to interpolation.

Table II (cont.) Calibration and Recovery Data for New Jersey Soil

ABC				CGA-265378			
Sample Code	Plot	Soil	Sample	Lab PPM	Sample PPM	Analysis PPM	on a Wet Percent Basis Recovery
Time Point	Plot	Soil Depth	Rep. No.	Spike Level	Extract Date	Analysis Date	Dil. Factor
			42162				
TIB. NJ. TR. 00-06*	A, B & C	1 con	3/14/96	03/15/96	3	1	0 0.0000
TIB. NJ. TR. 00-06*	A, B & C	2 con	3/14/96	03/16/96	4	1	0 0.0000
TIB. NJ. TR. 00-06*	A, B & C	3 0.01	3/14/96	03/16/96	5	1	404 0.0057 57
TIB. NJ. TR. 00-06*	A, B & C	4 0.01	3/14/96	03/16/96	6	1	542 0.0082 82
TIB. NJ. TR. 00-06*	A, B & C	5 0.01	3/14/96	03/16/96	8	1	487 0.0072 72
TIB. NJ. TR. 00-06*	A, B & C	6 0.01	3/14/96	03/16/96	9	1	564 0.0086 86
TIB. NJ. TR. 00-06*	A, B & C	7 0.1	3/14/96	03/16/96	10	1	4493 0.0776 78
TIB. NJ. TR. 00-06*	A, B & C	8 0.1	3/14/96	03/16/96	11	1	3264 0.0911 91
TIB. NJ. TR. 00-06*	A, B & C	9 1	3/14/96	03/16/96	13	1	433 0.0063 1
TIB. NJ. TR. 00-06*	A, B & C	9 1	3/14/96	03/16/96	14	10	0 0.0000 Diluted for CGA-173506
TIB. NJ. TR. 00-06*	A, B & C	10 1	3/14/96	03/16/96	15	1	442 0.0064 1
TIB. NJ. TR. 00-06*	A, B & C	10 1	3/14/96	03/16/96	16	10	0 0.0000 Diluted for CGA-173506
Reagent Blank		11	3/14/96	03/16/96	17	1	0 0.0000
Final Vol. = 5 mL Sam. Wt. = 20g MC Ch. #13 File: 001ANI							
µg/mL Comp.: CGA-265378							
					1	14248 0.9956	
					2	0.5 7285 0.3064 r = 0.9990	
					7	0.2 2998 0.2052 m = 14233	
					12	0.2 2961 0.2026 b = 77	
					18	0.05 715 0.0448	
					19	0.02 297 0.0155	

Sample #'s 9 and 10 are fortified with CGA-173506 only. They are calculated for % conversion for the other compounds.

Table II (cont.)

Calibration and Recovery Data for New Jersey Soil

Sample Code	ABC	Lab. PPM	Sample	Sample	Analysis Num.	Dilution Factor	Conc. on a Wet Weight Basis	Recovery
TIB-NJ-TR-00-06-A, B & C-16con	3/14/96	03/15/96	3	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-2con	3/14/96	03/16/96	4	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-3.5con	3/14/96	03/16/96	5	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-4con	3/14/96	03/16/96	6	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-5con	3/14/96	03/16/96	8	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-6con	3/14/96	03/16/96	9	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-7con	3/14/96	03/16/96	10	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-8con	3/14/96	03/16/96	11	1	0.5	0.0000	100	100
TIB-NJ-TR-00-06-A, B & C-9con	3/14/96	03/16/96	13	2	1.0	0.8803	100	100
TIB-NJ-TR-00-06-A, B & C-9.5con	3/14/96	03/16/96	14	10	7.990	0.8670	87	87
TIB-NJ-TR-00-06-A, B & C-10con	3/14/96	03/16/96	15	1	1.0	0.9258	100	100
Reagent Blank								
Sample #'s 9 and 10 are fortified with CGA-173506 only. They are calculated for % conversion for the other compounds.								

Sample #9 and 10 are fortified with CGA-173506 only. They are calculated for % conversion for the other compounds.

Final Vol. = 5 mL Sam. Wt. = 20g MC Ch. #16 File: 001ANI
µg/mL Comp.: CGA-173506

Table III (cont.) Calibration and Recovery Data for Georgia Soil

Sample Code	Pilot Plot	Soil Depth	Rep.	Lab No.	PPM Sample Spike Extract	Sample Analysis Date	Ingestion Number	PPM on a Wet Percent Basis	Height Recovery
Time Point	Site Ident	42163	Level						
TIB, GA, BS, UT, 00-06** A, B & C, 1, con.				3/14/96	03/16/96	3		0.0 0.0000	100
TIB, GA, BS, UT, 00-06** A, B & C, 2, con.				3/14/96	03/16/96	4		0.0 0.0000	100
TIB, GA, BS, UT, 00-06** A, B & C, 3, 0.01				3/14/96	03/16/96	5		788 0.0113	113
TIB, GA, BS, UT, 00-06** A, B & C, 4, 0.01				3/14/96	03/16/96	6		805 0.0114	114
TIB, GA, BS, UT, 00-06** A, B & C, 5, 0.01				3/14/96	03/16/96	8		812 0.0115	115
TIB, GA, BS, UT, 00-06** A, B & C, 6, 0.01				3/14/96	03/16/96	9		742 0.0108	108
TIB, GA, BS, UT, 00-06** A, B & C, 7, 0.				3/14/96	03/16/96	10		8629 0.0917	92.5
TIB, GA, BS, UT, 00-06** A, B & C, 8, 0.1				3/14/96	03/16/96	11		8636 0.0917	92.5
TIB, GA, BS, UT, 00-06** A, B & C, 9, 0.1				3/14/96	03/16/96	13		66965 0.6898	Over curve
TIB, GA, BS, UT, 00-06** A, B & C, 9, 1.314/96				03/17/96		14		7127 0.7625	76
TIB, GA, BS, UT, 00-06** A, B & C, 10, 1.314/96				03/17/96		15		74380 0.7658	Over curve
TIB, GA, BS, UT, 00-06** A, B & C, 10, 3/14/96				03/17/96		16		7251 0.7752	78
TIB, GA, BS, UT, 00-06** A, B & C, 11, 3/14/96				03/17/96		17		0.0 0.0000	
Reagent Blank									
TIB, GA, BS, UT, 00-06** A, B & C, 9 and 10 are fortified with CGA-173506 only.									
They are calculated for % conversion for the other compounds.									

a Multichrom values differ by ± 0.0001 ppm due to rounding.
 b Multichrom values differ by ± 0.0001 ppm due to rounding.

Table IV Summary Data for Fortified Soils

<u>% Recovery for CGA-339833</u>		
<u>Fortification Level (ppm)</u>	<u>New Jersey</u>	<u>Georgia</u>
0.010	100	115
0.010	86	125
0.010	91	109
0.010	94	107
0.10	109	94
0.10	115	98

<u>Pooled Recovery Data for all Soils by Fortification Level</u>		
	<u>0.010 ppm</u>	<u>0.10 ppm</u>
Average	103	104
Standard Deviation	13	9.7
Relative Standard Deviation	13	9.3
Range	86 to 125	94 to 115
Number of Samples	8	4

Table IV (con't) Summary Data for Fortified Soils

<u>% Recovery for CGA-192155</u>					
Fortification Level (ppm)	New Jersey		Georgia		Mean
	Mean	S.D.	Mean	S.D.	
0.010	96	31.0	102	10.0	99
0.010	69	30.0	109	10.0	89
0.010	69	30.0	94	10.0	82
0.010	52	20.0	89	10.0	71
0.10	97	31.0	101	10.0	99
0.10	103	61.0	105	10.0	102

<u>Pooled Recovery Data for all Soils by Fortification Level</u>					
Fortification Level	Average	Standard Deviation	Relative Standard Deviation %	Range	Number of Samples
0.010 ppm	85	20	23.4	52 to 109	8
0.10 ppm	102	10	9.7	97 to 105	4

Table IV (con't) Summary Data for Fortified Soils

<u>% Recovery for CGA-265378</u>		
Fortification Level (ppm)	New Jersey	Georgia
0.010	57	100
0.010	82	100
0.010	72	104
0.010	86	95
0.10	78	91
0.10	91	90


Pooled Recovery Data for all Soils by Fortification Level

	0.010 ppm	0.10 ppm
Average	87	88
Standard Deviation	16	6.4
Relative Standard Deviation	18	7.3
Range	57 to 104	78 to 91
Number of Samples	8	4


Table IV (con't) Summary Data for Fortified Soils

<u>% Recovery for CGA-173506</u>					
Fortification Level (ppm)	New Jersey		Georgia		
	Mean	S.E.	Mean	S.E.	S.E.
0.010	88	0.00.0	113		
0.010	108	0.00.0	114		
0.010	100	0.00.0	115		
0.010	109	0.00.0	108		
0.10	84	0.00.0	92		
0.10	91	0.00.0	92		
1.0	87		76		
1.0	91		78		
<u>Pooled Recovery Data for all Soils by Fortification Level</u>					
0.010 ppm		0.010 ppm		0.10 ppm	1.0 ppm
Average	107		90.2		83
Standard Deviation	9.0		3.9		7.2
Range	88 to 115		84 to 92		76 to 91
Number of Samples	8		4		4

Figure 1. Chemical Structures

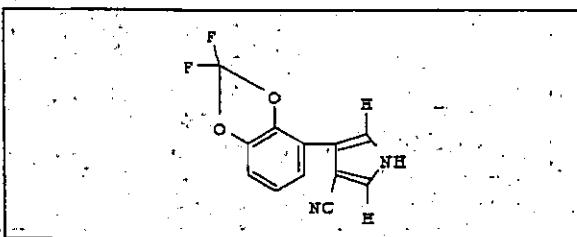Figure 1
Structure of CGA-173506

Ciba Code: CGA-173506
Molecular Formula: C₁₂H₁₄F₂N₂O₄
Molecular Weight: 248.191
CAS Number: 131341-86-1
CAS Name: 1H-Pyrrole-3-carbonitrile, 4-(2,2-difluoro-1,3-benzodioxol-4-yl)-

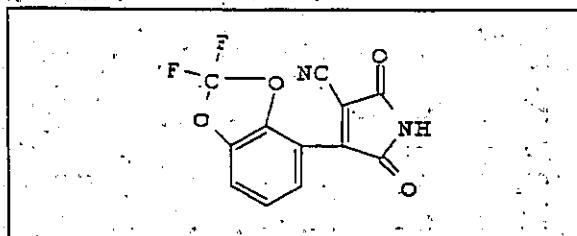Figure 2
Structure of CGA-265378

Ciba Code: CGA-265378
Molecular Formula: C₁₂H₁₄F₂N₂O₄
Molecular Weight: 278.173
CAS Number: not assigned
IUPAC Name: 4-(2,2-Difluoro-benzo[1,3]dioxol-4-yl)-2,5-dioxo-2,5-dihydro-1H-pyrrole-3-carbonitrile

Figure 1.(con't) Chemical Structures

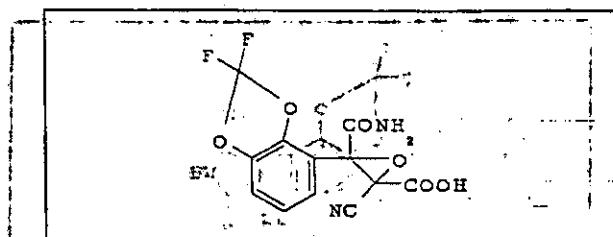


Figure 3
Structure of CGA-339833

Ciba Code: CGA-339833
Molecular Formula: C₁₂H₁₄F₂N₂O₆
Molecular Weight: 312.188
CAS Number: not assigned
CAS Name: Oxiranecarboxylic acid, 3-(aminocarbonyl)-2-cyano-3-(2,2-difluor-1,3-benzodioxol-4-yl)-, cis

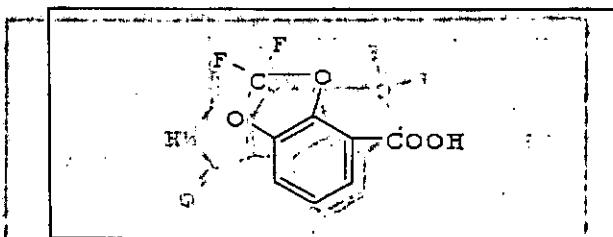


Figure 4
Structure of CGA-192155

Ciba Code: CGA-192155
Molecular Formula: C₁₂H₁₄F₂O₄
Molecular Weight: 202.115
CAS Number: 126120-85-2
CAS Name: 1,3-Benzodioxole-4-carboxylic acid, 2,2-difluor-

Figure 2. Extraction and Analysis Scheme

Weigh 20 g matrix into a 250 mL polyethylene bottle
(Fortify if required)

Add 100 mL of 90 ACN:9 H₂O:1 HOAc with 50 mg/L BHT

Shake at 280 oscillations/min (high) for 10 minutes

Balance opposing bottles with extraction solvent

Centrifuge 2 minutes @ 3000 rpm to remove suspended soil

Decant liquid through a glass wool plugged powder funnel into a 500 mL flat bottom

Extract a second 10 minute period with 50 mL of extraction solvent

Balance opposing bottles with extraction solvent

Centrifuge 2 minutes @ 3000 rpm to remove suspended soil

Decant liquid through the same glass wool plugged powder funnel into the same 500 mL flat bottom

Rotary evaporate the extraction liquids in the 500 mL flat bottom to 0.5 to 1 mL using a 20 to 40 °C water bath

Transfer the remaining liquid to a 15 mL graduated centrifuge tube

Pipet 2 mL of ACN to the 500 mL flat bottom and sonicate while rotating the flask to bring all previously wetted surfaces into contact with the ACN and transfer this completely to the 15 mL centrifuge tube

Use 2 mL of reagent grade water to wash and complete the transfer, then bring the volume to 5 mL for the extract

Vortex the 15 mL tube and then centrifuge to clarify.

Sample extract is ready to inject for CGA-265378 and CGA-173506 onto a column switching HPLC with UV detection

Transfer 3 mL of the extract to a 15 mL graduated tube and take the volume to 1.0 to 1.5 mL with a stream of nitrogen

Add reagent grade water to make a 1.5 mL volume

Sample extract is ready to inject for CGA-339833 and CGA-192155 onto a column switching HPLC with UV detection

Figure 3: Hydraulic Schematic for the HPLC System Used in ABC Method # CGA011696

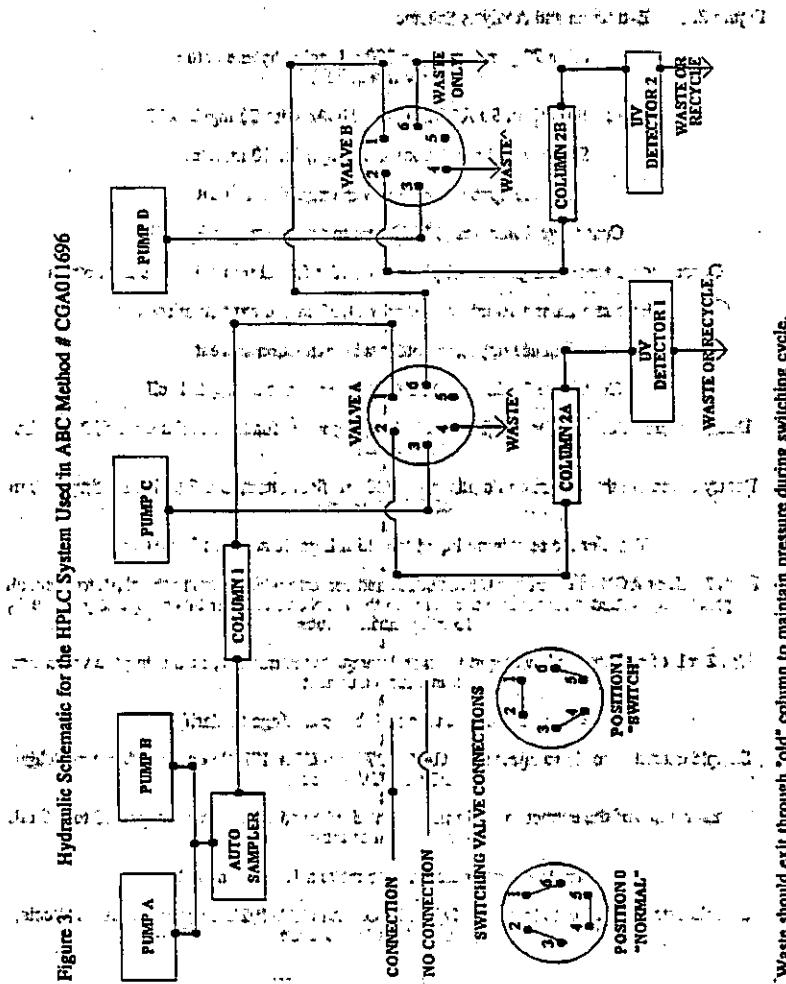


Figure 4. Example Chromatogram of Analytics on a SB-CN Column Using 40% ACN: 60% Reagent Grade Water with 5 mM/L HOAc at 1 mL/minute

