

Cover Sheet for

Environmental Chemistry Method

Pesticide Name: Penoxsulam

MRID#: 458308-08

Matrix: Soil

Analysis: LC/MS/MS

This method is provided to you by the Environmental Protection Agency's (EPA) Environmental Chemistry Laboratory (ECL). This method *is not* an EPA method but one which was submitted to EPA by the pesticide manufacturer to support product registration. EPA recognizes that the methods may be of some utility to state, tribal, and local authorities, but makes no claim of validity by posting these methods. Although the Agency reviews *all* Environmental Chemistry Methods submitted in support of pesticide registration, the ECL evaluates only about 30% of the currently available methods in the laboratory. Most methods perform satisfactorily but some, particularly the older methods, have deficiencies. Moreover, the print quality of the methods varies considerably because the methods originate from different sources. Therefore, the methods offered represent the best available copies.

If you have difficulties in downloading the method, or further questions concerning the methods, you may contact Elizabeth Flynt at 228-688-2410 or via e-mail at flynt.elizabeth@epa.gov.

GRM: 01.31
EFFECTIVE: July 13, 2002
SUPERSEDES: NA




Determination of Residues of XDE-638 and Metabolites in Soil and Sediment
by Liquid Chromatography with Tandem Mass Spectrometry

M. J. Hastings and G. E. Schelle

1. SCOPE

This method is applicable for the quantitative determination of XDE-638 and its metabolites in soil and sediment. The method measures XDE-638, the 5-OH, BSTCA, BSA, sulfonamide, and the 2-amino-TP metabolites over the concentration range 3.0-100 ng/g with a validated limit of quantitation of 3.0 ng/g. Chemical names and structures for these compounds are given in Table 1.

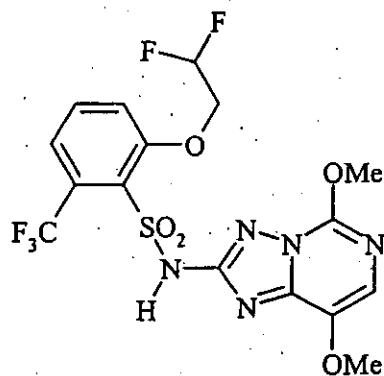

XDE-638
CAS No: 219714-96-2

2. PRINCIPLE

Residues of XDE-638 and its metabolites are extracted from soil or sediment using an acetonitrile:1.0 N hydrochloric acid solution (90:10 v/v). An aliquot of the extract is concentrated to remove the acetonitrile and then diluted with 0.1 N hydrochloric acid. The extract is purified using an HLB solid-phase extraction plate (SPE). The SPE plate is washed with a water:methanol solution (95:5 v/v) before XDE-638 and its metabolites are eluted from the SPE plate with an acetonitrile:methanol solution (80:20 v/v). The eluate is evaporated to dryness and reconstituted with a water:acetonitrile:methanol:acetic acid solution (90:5:5:0.1) containing a stable isotope of XDE-638 as internal standard (ISTD). The final solution is analyzed by liquid chromatography with tandem mass spectrometry (LC/MS/MS).

3. **SAFETY PRECAUTIONS**

- 3.1. Each analyst must be acquainted with the potential hazards of the reagents, products, and solvents used in this method before commencing laboratory work. SOURCES OF INFORMATION INCLUDE MATERIAL SAFETY DATA SHEETS, LITERATURE, AND OTHER RELATED DATA. Safety information on non Dow AgroSciences LLC products should be obtained from the container label or from the supplier. Disposal of reagents, reactants, and solvents must be in compliance with local, state, and federal laws and regulations.
- 3.2. Acetonitrile and methanol are flammable and volatile and should be used in well-ventilated areas away from ignition sources.
- 3.3. Acetic acid and hydrochloric acid are corrosive and can cause severe burns. It is imperative that proper eye and personal protection equipment be worn when handling these chemicals.

4. **EQUIPMENT** (Note 12.1)

4.1. **Laboratory Equipment**

- 4.1.1. Balance, analytical, Model AE100, Mettler Instrument Corporation, Hightstown, NJ 08520.
- 4.1.2. Balance, analytical, Model P-1200, Mettler Instrument Corporation.
- 4.1.3. Centrifuge, with rotor to accommodate 40-mL vials, Model Centra-GP8, International Equipment Company, Needham Heights, MA 02194.
- 4.1.4. Evaporator, TurboVap LV, Zymark Corporation, Hopkinton, MA 01748.
- 4.1.5. Hammer mill, with 3/16-inch screen, Model 2001, AGVISE Laboratories, Inc., Northwood, ND 58267.
- 4.1.6. Oven, Model OV-490A-2, Blue M Electric Company, Blue Island, IL 60406.
- 4.1.7. Pipetter, adjustable, Eppendorf, 10-100 μ L, catalog number 05-402-48, Fisher Scientific, Pittsburgh, PA 15275.
- 4.1.8. Pipetter, adjustable, Eppendorf, 50-1000 μ L, catalog number 21-378-83, Fisher Scientific.
- 4.1.9. Shaker, Model 6010, Eberbach Corporation, Ann Arbor, MI 48106.

- 4.1.10. Ultrasonic cleaner, Model 1200, Branson Cleaning Equipment Company, Shelton, CT 06484.
- 4.1.11. Vacuum manifold, 96-Well, catalog number 121-9601, International Sorbent Technology Ltd, Hengoed, Mid Glamorgan UK and distributed by Jones Chromatography USA, Inc., Lakewood, CO 80228.
- 4.1.12. Vortex mixer, Model G-560, Scientific Industries, Inc., Bohemia, NY 11716.

4.2. Chromatographic Equipment (Note 12.1.)

- 4.2.1. Column, analytical, ZORBAX SB-C8, 4.6 x 75 mm, 3.5- μ m, catalog number 866953-906, Agilent Technologies, Wilmington, DE 19808.
- 4.2.2. Liquid chromatograph autosampler, Model 1100, Agilent Technologies.
- 4.2.3. Liquid chromatograph binary pump, Model 1100, Agilent Technologies.
- 4.2.4. Liquid chromatograph degasser, Model 1100, Agilent Technologies.
- 4.2.5. Mass spectrometer, Model API 3000, Applied Biosystems, Foster City, CA 94404.
- 4.2.6. Mass spectrometer data system, Analyst 1.1, Applied Biosystems.

5. GLASSWARE AND MATERIALS (Note 12.1)

- 5.1. Adsorbent, drierite, indicating, catalog number 07-578-4A, Fisher Scientific.
- 5.2. Bottle, 1.0-L PyrexPlus media bottle, catalog number 06-423-3D, Fisher Scientific.
- 5.3. Bottle, 2.0-L PyrexPlus media bottle, catalog number 06-423-3E, Fisher Scientific.
- 5.4. Cylinder, graduated mixing, 50-mL catalog number 20039-0050, Kimble/Kontes, Vineland, NJ 08360.
- 5.5. Cylinder, graduated mixing, 100-mL catalog number 20039-0100, Kimble/Kontes, Vineland, NJ 08360.
- 5.6. Cylinder, graduated, 500-mL, catalog number C7000-500, National Scientific Company, Lawrenceville, GA 30243.
- 5.7. Cylinder, graduated, 1000-mL, catalog number C7000-1L, National Scientific Company.

- 5.8. Cylinder, graduated, 2000-mL, catalog number C7000-2L, National Scientific Company.
- 5.9. Deep-well collection plate, catalog number 121-5203, International Sorbent Technology Ltd.
- 5.10. Desiccator, Glass, 250 mm I.D., catalog number 08-595-E, Fisher Scientific.
- 5.11. Dish, 42-mL aluminum weighing, catalog number 08-732, Fisher Scientific.
- 5.12. Flask, volumetric, 10-mL, catalog number 161-8986, National Scientific Company, Duluth, GA 30097.
- 5.13. Flask, volumetric, 100-mL, catalog number 161-8987, National Scientific Company, Duluth, GA 30097.
- 5.14. Pipet, 5-mL disposable seriological, catalog number, 13-666-7D, Fisher Scientific.
- 5.15. Pipet, 3.2-mL disposable transfer, catalog number, 13-711-7, Fisher Scientific.
- 5.16. Pipet, volumetric, 0.5-mL, catalog number 261-6010, National Scientific Company.
- 5.17. Pipet, volumetric, 1.0-mL, catalog number 261-6011, National Scientific Company.
- 5.18. Pipet, volumetric, 2.0-mL, catalog number 261-6012, National Scientific Company.
- 5.19. Pipet, volumetric, 3.0-mL, catalog number 261-6013, National Scientific Company.
- 5.20. Pipet, volumetric, 5.0-mL, catalog number 261-6015, National Scientific Company.
- 5.21. Pipet, volumetric, 10.0-mL, catalog number 261-6020, National Scientific Company.
- 5.22. Vial, autosampler, 2-mL, catalog number C4000-1, National Scientific Company.
- 5.23. Vial, scintillation, 20-mL, catalog number 03-337-7, Fisher Scientific.
- 5.24. Vial cap, for autosampler vial, catalog number C4000-54B, National Scientific Company.
- 5.25. Vial, 40-mL, with PTFE-lined screw cap, catalog number B7800-6, National Scientific Company.
- 5.26. Waters HLB SPE plate, 30-mg packing, catalog number WAT 058951, Waters, Milford, MA 01757.

6. REAGENTS, STANDARDS, AND PREPARED SOLUTIONS (Note 12.1.)

6.1. Reagents

- 6.1.1. Acetic acid, catalog number A38S-500, Fisher Scientific.
- 6.1.2. Acetonitrile, HPLC grade, catalog number 2856, Mallinkrodt Baker, Inc., Paris, KY 40361.
- 6.1.3. Hydrochloric acid, 0.1 N, catalog number SA54-1, Fisher Scientific.
- 6.1.4. Hydrochloric acid, 1.0 N, catalog number SA48-1, Fisher Scientific.
- 6.1.5. Methanol, HPLC grade, catalog number 3041, Mallinkrodt Baker Inc.
- 6.1.6. Water, HPLC grade, catalog number WX0004-1, Fisher Scientific.

6.2. Standards

- 6.2.1. 2-amino-TP metabolite of XDE-638: 5,8-dimethoxy[1,2,4]triazolo[1,5-c]pyrimidin-2-amine.
- 6.2.2. BSA triethylammonium salt of XDE-638: 2-(2,2-difluoroethoxy)-6-(trifluoromethyl)benzenesulfonic acid.
- 6.2.3. BSTCA triethylammonium salt of XDE-638: triethylammonium 5-[[[2-(2,2-difluoroethoxy)-6-(trifluoromethyl) phenyl]sulfonyl]amino]-1*H*-1,2,4-triazole-3-carboxylic acid.
- 6.2.4. 5-OH metabolite of XDE-638: 2-(2,2-difluoroethoxy)-*N*-(5,6-dihydro-8-methoxy-5-oxo[1,2,4]triazolo[1,5-c]pyrimidin-2-yl)-6-(trifluoromethyl)-benzenesulfonamide.
- 6.2.5. Sulfonamide metabolite of XDE-638: 2-(2,2-difluoroethoxy)-6-(trifluoromethyl)-benzenesulfonamide.
- 6.2.6. XDE-638: 2-(2,2-difluoroethoxy)-*N*-(5,8-dimethoxy[1,2,4]triazolo[1,5-c]pyrimidin-2-yl)-6-(trifluoromethyl)-benzenesulfonamide.

Compounds can be obtained from Test Substance Coordinator, Dow AgroSciences LLC, 9330 Zionsville Road, Building 304, Indianapolis, IN 46268-1054.

- 6.2.7. Stable isotope of XDE-638: 2-(2,2-difluoroethoxy)-N-(5,8-dimethoxy[1,2,4]triazolo[1,5-c]pyrimidin-2-yl-2-¹³C-3,4-¹⁵N₂)-6-(trifluoromethyl)-benzenesulfonamide.

Compound can be obtained from Specialty Synthesis Group, Dow AgroSciences LLC, 9330 Zionsville Road, Building 306, Indianapolis, IN 46268-1054.

6.3. Prepared Solutions

- 6.3.1. acetonitrile/1.0 N hydrochloric acid (90:10)

Measure 200 mL of 1.0 N hydrochloric acid into a 2.0-L bottle using a 500-mL graduated cylinder. Measure 1800 mL of acetonitrile using 2.0-L graduated cylinder and add to the bottle. Cap the bottle and mix. Allow the solution to equilibrate to room temperature.

- 6.3.2. acetonitrile:methanol:acetic acid (50:50:0.1)

Add 1.0 mL of acetic acid into a clean 1.0-L bottle. Measure 500 mL of acetonitrile using a graduated cylinder and add to the bottle. Measure 500 mL of methanol using a graduated cylinder and add to the bottle. Cap the bottle and mix. Allow the solution to equilibrate to room temperature before use.

- 6.3.3. acetonitrile:methanol (80:20)

Add 80 mL of acetonitrile and 20 mL of methanol to a 100-mL bottle using a measuring cylinder. Cap the bottle and mix the solution. Allow the solution to equilibrate to room temperature before use.

- 6.3.4. water:acetic acid (100:0.1)

Add 1.0 mL of acetic acid into a clean 1.0-L bottle. Measure 1.0 L of HPLC grade water using a graduated cylinder and add to the bottle. Cap the bottle and mix.

- 6.3.5. water:methanol solution (95:5 v/v)

Pipette 5.0 mL of methanol into a 100-mL volumetric flask and dilute to volume with water. Mix the solution and allow to equilibrate to room temperature before use.

- 6.3.6. water:acetonitrile:methanol:acetic acid (90:5:5:0.1)

Add 50 mL of methanol and 50.0 mL of acetonitrile into a clean 1.0-L bottle using a graduated cylinder. Pipette 1.0 mL of acetic acid into the bottle. Add 900 mL of water to the bottle using a graduated cylinder. Mix the solution and allow to equilibrate to room temperature before use.

7. PREPARATION OF STANDARD SOLUTIONS (Note 12.2.)

7.1. Preparation of Internal Standard Solution

- 7.1.1. Weigh 0.010 g of the stable-isotope labeled XDE-638 into a 20-mL vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.1.2. Pipette 1.0 mL from the 1000- μ g/mL solution prepared in Section 7.1.1. into a 10-mL volumetric flask and dilute to volume with acetonitrile to obtain an XDE-638 stable-isotope solution at 100.0 μ g/mL.
- 7.1.3. Pipet 1.0 mL of the 100- μ g/mL XDE-638 stable-isotope solution prepared in Section 7.1.2 into a 10-mL volumetric flask and dilute to volume with acetonitrile to obtain an XDE-638 stable-isotope solution at 10.0 μ g/mL.
- 7.1.4. Pipet 1.0 mL of the 10- μ g/mL XDE-638 stable-isotope solution prepared in Section 7.1.3 into a 10-mL volumetric flask and dilute to volume with acetonitrile to obtain an XDE-638 stable-isotope solution at 1.0 μ g/mL.
- 7.1.5. Pipet 5.0 mL of the 1.0 μ g/mL XDE-638 stable-isotope solution prepared in Section 7.1.4 into a 1.0-L volumetric flask. Add 50 mL of acetonitrile, 50 mL of methanol and 1.0 mL of acetic acid into the flask. Add approximately 850 mL of water into the flask. Swirl the flask and allow the solution to equilibrate to room temperature before diluting to volume with water to obtain a working XDE-638 stable-isotope solution at 0.005 μ g/mL.

7.2. Preparation of XDE-638 and Metabolites Spiking Solutions

- 7.2.1. Weigh 0.0100 g of 2-amino-TP of XDE-638 into a 20-mL scintillation vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.2.2. Weigh 0.0133 g of BSA triethylammonium salt of XDE-638 (equivalent to 0.01 g of the BSA metabolite) into a 20-mL scintillation vial and dissolve the compound in 10 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.2.3. Weigh 0.0139 g of BSTCA triethylammonium salt of XDE-638 (equivalent to 0.01 g of the BSTCA metabolite) into a 20-mL scintillation vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.2.4. Weigh 0.0100 g of 5-OH of XDE-638 into a 20-mL scintillation vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.2.5. Weigh 0.0100 g of sulfonamide of XDE-638 into a 20-mL scintillation vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.

- 7.2.6. Weigh 0.0100 g of XDE-638 into a 20-mL scintillation vial and dissolve the compound in 10.0 mL of acetonitrile to obtain a 1000- μ g/mL stock solution.
- 7.2.7. Pipette 1.0 mL from each of the 1000- μ g/mL solution prepared in Sections 7.2.1-7.2.6 into a 100-mL volumetric flask and dilute to volume with water:acetonitrile:methanol:acetic acid (90:5:5:0.1) to obtain a solution containing XDE-638, 5-OH, BSTCA, 2-amino-TP, BSA, and sulfonamide at 10.0 μ g/mL.
- 7.2.8. Pipette 10.0 mL of the 10.0- μ g/mL mixed standard prepared in section 7.2.7 into a 100-mL volumetric flask and dilute to volume water:acetonitrile:methanol:acetic acid (90:5:5:0.1) to obtain a solution containing XDE-638, 5-OH, BSTCA, 2-amino-TP, BSA, and sulfonamide at 1.0 μ g/mL.
- 7.2.9. Pipette 10.0 mL of the 1.0- μ g/mL mixed standard prepared in section 7.2.8 into a 100-mL volumetric flask and dilute to volume with water:acetonitrile:methanol:acetic acid (90:5:5:0.1) to obtain a solution containing XDE-638, 5-OH, BSTCA, 2-amino-TP, BSA, and sulfonamide at 0.1 μ g/mL.

7.3. Preparation of XDE-638 and Metabolites Calibration Solutions

Prepare calibration standard solutions in water:acetonitrile:methanol:acetic acid (90:5:5:0.1) from the 10.0- μ g/mL mixed standard (Section 7.1.7) over the range 0.00025–0.05 μ g/mL as described below.

Original Standard Concentration μ g/mL	Aliquot of Original Standard mL	Final Soln. Volume mL	Calib Soln. Final Conc. μ g/mL	Equivalent Sample Conc. ng/g
10.00	10.0	100	1.00	N/A
1.00	10.0	100	0.10	N/A
1.00	5.0	100	0.05 ^a	266.7
1.00	3.5	100	0.035 ^a	186.7
1.00	2.0	100	0.02 ^a	106.7
0.10	10.0	100	0.01 ^a	53.3
0.10	5.0	100	0.005 ^a	26.7
0.10	1.0	100	0.001 ^a	5.3
0.10	0.5	100	0.0005 ^a	2.7
0.10	0.25	100	0.00025 ^a	1.4

^a Add 0.5 mL of a 1.0- μ g/mL XDE-638 stable isotope internal standard solution (prepared in Section 7.1.4.) to each volumetric flask prior to making to volume with mobile phase to give calibration standards containing 0.005 μ g/mL of XDE-638 stable-isotope internal standard.

8. LIQUID CHROMATOGRAPHY/TANDEM MASS SPECTROMETRY (LC/MS/MS)

8.1. Typical Liquid Chromatography Operating Conditions (Note 12.3.)

Instrumentation: Agilent Model 1100 autosampler
Agilent Model 1100 binary pump
Agilent Model 1100 degasser
PE SCIEX API 3000 LC/MS/MS System
PE SCIEX Analyst 1.1 data system

Column: Zorbax SB C8
4.6 x 75 mm, 3.5- μ m

Column Temperature: 35 °C

Injection Volume: 40 μ L

Run Time: 16 minutes

Mobile Phase: A –methanol:acetonitrile with 0.1% acetic acid
B –water with 0.1% acetic acid

Flow Rate: 900 μ L/min, 150 μ L/min split to ESI source

Gradient:	Time, min	A, %	B, %
	0.0	10	90
	0.5	10	90
	13.0	90	10
	13.1	10	90
	16.0	10	90

8.2. Typical Mass Spectrometry Operating Conditions

API 3000:

Interface: TurboIonSpray
Scan Type: MRM
Resolution: Q1 – unit, Q3 – low
Curtain Gas (CUR): 14
Collision Gas (CAD): 4.0
Temperature (TEM): 425 °C
Ion Source Gas 1 (GS1): 10
Ion Source Gas 2 (GS2): 7000
Period 1
Time: 6.25 minutes

Polarity: Positive
IonSpray Voltage (IS) 5500

Compound	<u>Ion m/z</u>	Time, ms	CE, v
2-amino-TP	Q1 196.1 Q3 181.2	150	29

Period 2

Time: 3.50 minutes
Polarity: Negative
IonSpray Voltage (IS) -4300

Compound	<u>Ion m/z</u>	Time, ms	CE, v
5-OH	Q1 468.0 Q3 385.8	150	-26
BSTCA	415.0 329.0	150	-22
BSA	305.0 176.0	150	-40
Sulfonamide	304.0 78.0	150	-48

Period 3

Time: 3.25 minutes
Polarity: Positive
IonSpray Voltage (IS) 5500

Compound	<u>Ion m/z</u>	Time, ms	CE, v
XDE-638	Q1 484.0 Q3 195.0	150	37
Stable Isotope of XDE-638	487.0 198.0	150	37

8.3. Typical Mass Spectra

Typical mass spectra and product ion spectra of XDE-638, metabolites of XDE-638, and internal standard are presented in Figures 1-7.

8.4. Typical Calibration Curve

Typical calibration curves for the determination of XDE-638 and metabolites of XDE-638 in soil are shown in Figures 8-13.

8.5. Typical Chromatograms

Typical chromatograms for a calibration standard, control soil extract, and control soil extracts fortified at limit of quantitation 3.0 ng/g (LOQ) and the highest fortified level are presented in Figures 14-17.

9. DETERMINATION OF RECOVERY OF XDE-638 AND METABOLITES IN SOIL AND SEDIMENT

9.1 Method Validation

Unless otherwise specified, a sample set should contain the following samples:

- At least one reagent blank.
- At least one control.
- At least one control fortified at the limit of detection.
- At least two controls fortified at the limit of quantitation.
- At least one control fortified at a higher concentration.

9.2 Sample Preparation

Prepare soil samples for analysis by freezing the soil with dry ice and then grinding or chopping with a hammer mill equipped with a 3/16-inch screen size. For sediment samples, thoroughly stir the sediment prior to use.

9.3. Sample Analysis for XDE-638 and Metabolites

- 9.3.1. Weigh 5 ± 0.1 g portions of the control soil or sediment into a series of 40-mL vials. For preparing fortified samples, add appropriate aliquots of the appropriate spiking solutions to obtain concentrations ranging from 1.0 to 100 ng/g.
- 9.3.2. Add 25 mL of the acetonitrile/1.0 N hydrochloric acid (90:10) extraction solution to each sample vial. Cap the vial with a PTFE-lined cap.
- 9.3.3. Shake the sample vial for a minimum of 60 minutes on a reciprocating shaker at approximately 180 excursions/minute.
- 9.3.4. Centrifuge the sample vial for approximately 5 minutes at 2000 rpm.
- 9.3.5. Decant the extraction solution into a clean 50-mL graduated cylinder.
- 9.3.6. Add an additional 15 mL of the acetonitrile/1.0 N hydrochloric acid (90:10) extraction solution to each sample vial.
- 9.3.7. Cap the vial with a PTFE-lined cap and vortex the sample to break loose the soil layer formed during centrifugation.
- 9.3.8. Shake the sample vial for a minimum of 30 minutes on a reciprocating shaker at approximately 180 excursions/minute. Centrifuge the sample vial for approximately 5 minutes at 2000 rpm.

- 9.3.9. Decant the soil extract to the cylinder from Step 9.3.5 and adjust final volume to 40.0 mL with additional extraction solution and mix thoroughly.
- 9.3.10. Transfer a 4.0-mL aliquot of the extraction solution from Step 9.3.9 into a clean 40-mL vial.
- 9.3.11. Evaporate the extracts to near dryness (approximately 50-100 µL should remain in the vial) using a TurboVap evaporator set at 40 °C and a nitrogen pressure of 20 psi.

Do not evaporate to dryness. Remove each vial from the evaporator as soon as evaporation is complete.

- 9.3.12. Add 4.0 mL of 0.1 N hydrochloric acid to each vial, vortex mix and sonicate for approximately 30 seconds.
- 9.3.12.1. Purify the samples using the following SPE procedure (Note 12.4.):
 - a. Condition a Waters HLB 96-well plate (30-mg) with 0.2 mL of methanol followed by 1.0 mL of 0.1 N hydrochloric acid (dry the plate under full vacuum for 10 seconds between solvents).
 - b. Transfer 1.50 mL of the sample solution from Step 9.3.10 to the 96-well plate. Draw the sample through the plate at approximately 1 mL/min, discarding the eluate. Dry the plate under full vacuum for 10 seconds after sample has eluted.
 - c. Wash the plate with 1.0 mL of water:methanol solution (95:5 v/v), discarding the eluate. Dry the plate under full vacuum for 10 seconds after the sample has all passed through the plate.
 - d. Elute the XDE-638 and metabolites from the plate at approximately 1 mL/min with two 1.0-mL aliquots of acetonitrile:methanol (80:20), collecting the eluate in a 2-mL deep well rack. (Allow the elution solvent to soak on the plate for approximately 30 seconds before elution.)

- 9.3.13. Using a transfer pipet, transfer the extracts to a clean 40-mL vial and evaporate the extracts to dryness using a TurboVap evaporator set at 40 °C and a nitrogen pressure of 10 psi.

Immediately remove the sample from the evaporator when completely dry.

- 9.3.14. Reconstitute the samples in 1.0 mL of 0.005-µg/mL XDE-638 stable-isotope internal standard in methanol:acetonitrile:water:acetic acid (5:5:90:0.1). Sonicate and vortex mix the sample vials for approximately 30 seconds.
- 9.3.15. Transfer the samples and standards to a 2-mL autosampler vial and seal with a cap.

- 9.3.16. Analyze the sample along with the calibration standards using the LC/MS/MS conditions listed in Section 8. For samples which contain XDE-638 and metabolite concentrations >0.05 µg/mL dilute with the 0.005-µg/mL XDE-638 stable-isotope internal standard in methanol:acetonitrile:water:acetic acid (5:5:90:0.1) to give a concentration <0.05 µg/mL. Determine the suitability of the chromatographic system using the following criteria:
- Standard curve linearity: Determine that the correlation coefficient equals or exceeds 0.995 for the least squares equation which describes the detector response as a function of standard curve concentration.
 - Appearance of chromatograms: Visually determine that the chromatograms resemble those shown in Figures 14-17 with respect to peak response, baseline noise, and background interference. Visually determine that a minimum signal-to-noise ratio of 5:1 has been attained for the 0.00025-µg/mL calibration standard (equivalent to approximately 1.5 ng/g of analyte in soil or sediment).

10. CALCULATIONS

10.1. Calculation of Percent Recovery for XDE-638

- 10.1.1. Inject a series of calibration standards (Section 7.3.) as described in Section 8 and determine the peak areas for the analyte and the internal standard as indicated below.

XDE-638	<i>m/z</i> Q1/Q3 484/195 (quantitation)
XDE-638 stable isotope	<i>m/z</i> Q1/Q3 487/198 (internal standard)

- 10.1.2. For each standard, calculate the quantitation ratio. For example, using the data for XDE-638 from Figure 14 (f):

$$\begin{aligned}\text{Quantitation ratio} &= \frac{\text{peak area of quantitation ion}}{\text{peak area of internal standard ion}} \\ \text{Quantitation ratio} &= \frac{\text{peak area for } m/z \text{ Q1/Q3 484/195}}{\text{peak area for } m/z \text{ Q1/Q3 487/198}} \\ \text{Quantitation ratio} &= \frac{9.89e3}{8.41e4} \\ \text{Quantitation ratio} &= 0.118\end{aligned}$$

- 10.1.3. Prepare a standard curve by plotting the ratio of the concentrations of the analyte/internal standard on the abscissa (x-axis) and the respective quantitation ratio on the ordinate (y-axis) as shown in Figure 8. Using linear regression analysis (13.1.) forced through zero (Note 12.5.), determine the equation for the curve with respect to the abscissa.

For example, using linear regression with the XDE-638 data from Figure 8:

$$X = \left(\frac{Y - \text{intercept}}{\{\text{slope/int std conc}\}} \right)$$

$$\text{XDE - 638 conc.} \quad (\mu\text{g/mL}) = \left(\frac{\text{XDE - 638 quantitation ratio} - \text{intercept}}{\{1.19/0.005\}} \right)$$

$$\text{XDE - 638 conc.} \quad (\mu\text{g/mL}) = \left(\frac{\text{XDE - 638 quantitation ratio} - 0}{238} \right)$$

10.2. Calculation of Percent Recovery for XDE-638

- 10.2.1. Determine the gross concentration in each recovery sample by substituting the quantitation ratio obtained into the above equation and solving for the concentration.

For example, using the data for XDE-638 from Figure 16f:

$$\text{XDE - 638 conc.} \quad (\text{gross } \mu\text{g/mL}) = \left(\frac{\text{XDE - 638 quantitation ratio} - 0}{238} \right)$$

$$\text{XDE - 638 conc.} \quad (\text{gross } \mu\text{g/mL}) = \left(\frac{0.11486 - 0}{238} \right)$$

$$\text{XDE - 638 conc.} \quad (\text{gross } \mu\text{g/mL}) = 0.000483 \mu\text{g/mL}$$

Convert the concentration of $\mu\text{g/mL}$ to ng/g as follows:

$$\text{XDE - 638 conc.} \quad (\text{gross ng/g}) = 0.000483 \mu\text{g/mL} \times \frac{(40 \text{ mL}/1.5 \text{ mL}) \times 1000}{5 \text{ g}}$$

$$\text{XDE - 638 conc.} \quad (\text{gross}) = 2.58 \text{ ng/g}$$

- 10.2.2. Determine the net concentration in each recovery sample by subtracting the apparent XDE-638 concentration in the control sample from that of the gross XDE-638 concentration in the recovery sample.

For example, using the data from Figure 15f and 16f:

$$\text{XDE-638 conc.} = \frac{\text{XDE-638 conc.} - \text{XDE-638 conc.}}{\text{(net ng/g)} \quad \text{(gross ng/g)} \quad \text{(control ng/g)}}$$

$$\text{XDE-638 conc.} = \frac{2.58 \text{ ng/g} - 0.0 \text{ ng/g}}{\text{(net ng/g)}}$$

$$\text{XDE-638 conc.} = \frac{2.58 \text{ ng/g}}{\text{(net)}}$$

- 10.2.3. Determine the percent recovery by dividing the net concentration of each recovery sample by the concentration added.

$$\text{Recovery} = \frac{\text{Conc. Found}}{\text{Conc. Added}} \times 100\%$$

$$\text{Recovery} = \frac{2.58}{3.00} \times 100\%$$

$$\text{Recovery} = 86\%$$

10.3. Determination of XDE-638 Residues in Soil or Sediment

- 10.3.1. Determine the gross concentration in each treated sample by substituting the quantitation ratio obtained into the equation for the standard calibration curve, and calculating the uncorrected residue result as described in Sections 10.2.1 and 10.2.2.

- 10.3.2. For those analytes that require correction for method recovery, use the average recovery of all the recovery samples from a given sample set to correct for method efficiency.

For example, using the XDE-638 data from Figure 16f and the average recovery from Table 2 for the sample analyzed on 04-Dec-2001:

$$\text{XDE-638 conc.} = \frac{\text{XDE-638 conc.} \times \left(\frac{100}{\text{Average \% recovery}} \right)}{\text{(corrected ng/g)} \quad \text{(gross ng/g)}}$$

$$\text{XDE-638 conc.} = \frac{2.58 \text{ ng/g} \times \frac{100}{83}}{\text{(corrected ng/g)}}$$

$$\text{XDE-638 conc.} = 3.11 \text{ ng/g}$$

(corrected ng/g)

10.4. Calculation of Percent Recovery for 5-OH Metabolite, Sulfonamide, BSTCA, BSA, and 2-Amino-TP

- 10.4.1. Inject a series of calibration standards as described in Section 8 and determine the peak areas for the analytes.

5-OH of XDE-638	<i>m/z</i> Q1/Q3 468/386
sulfonamide of XDE-638	<i>m/z</i> Q1/Q3 304/78
BSTCA of XDE-638	<i>m/z</i> Q1/Q3 415/329
BSA of XDE-638	<i>m/z</i> Q1/Q3 305/176
2-Amino-TP of XDE-638	<i>m/z</i> Q1/Q3 196/181

- 10.4.2. Prepare a standard curve by plotting the concentration of the analyte on the abscissa (x-axis) and the respective peak area on the ordinate (y-axis) as shown in Figure 9-13. Using linear regression analysis forced through zero, determine the equation for the curve with respect to the abscissa.

For example, using linear regression (13.1.) with the data from Figure 9:

$$X = \left(\frac{Y - \text{intercept}}{\text{slope}} \right)$$

$$5\text{-OH conc.} = \left(\frac{5\text{-OH peak area} - \text{intercept}}{1.51e7} \right)$$

($\mu\text{g/mL}$)

$$5\text{-OH conc.} = \left(\frac{5\text{-OH peak area} - 0}{1.51e7} \right)$$

($\mu\text{g/mL}$)

10.5. Calculation of Percent Recovery for 5-OH Metabolite

- 10.5.1. Determine the gross concentration in each recovery sample by substituting the area obtained into the above equation and solving for the concentration.

For example, using the data for 5-OH metabolite from Figure 16e:

$$5\text{-OH conc.} = \left(\frac{5\text{-OH peak area} - 0}{1.51e7} \right)$$

(gross $\mu\text{g/mL}$)

$$5\text{-OH conc.} = \left(\frac{7.75e3 - 0}{1.51e7} \right)$$

$$5\text{-OH conc.} = 0.000513 \mu\text{g/mL}$$

Convert the concentration of $\mu\text{g/mL}$ to ng/g as follows:

$$5\text{-OH conc.} = 0.000513 \mu\text{g/mL} \times \frac{(40 \text{ mL}/1.5 \text{ mL}) \times 1000}{5 \text{ g}}$$

$$5\text{-OH conc.} = 2.74 \text{ ng/g}$$

- 10.5.2. Determine the net concentration in each recovery sample by subtracting the apparent 5-OH concentration in the control sample from that of the gross 5-OH metabolite concentration in the recovery sample.

For example, using the data from Figures 15e and 16e:

$$5\text{-OH conc.} = 5\text{-OH conc.} - 5\text{-OH conc.} \\ (\text{net ng/g}) \quad (\text{gross ng/g}) \quad (\text{control ng/g})$$

$$5\text{-OH conc.} = 2.74 \text{ ng/g} - 0.0 \text{ ng/g} \\ (\text{net ng/g})$$

$$5\text{-OH conc.} = 2.74 \text{ ng/g} \\ (\text{net ng/g})$$

- 10.5.3. Determine the percent recovery by dividing the net concentration of each recovery sample by the theoretical concentration added.

$$\text{Recovery} = \frac{\text{Conc. Found}}{\text{Conc. Added}} \times 100\%$$

$$\text{Recovery} = \frac{2.74 \text{ ng/g}}{3.0 \text{ ng/g}} \times 100\%$$

$$\text{Recovery} = 91\%$$

10.6. Determination of 5-OH Metabolite in Soil or Sediment

- 10.6.1. Determine the gross concentration in each treated sample by substituting the area obtained into the equation for the standard calibration curve, and calculating the uncorrected residue result as described in Sections 10.5.1 and 10.5.2.

For those analytes that require correction for method recovery, use the average recovery of all the recovery samples from a given sample set to correct for method efficiency.

For example, using 5-OH data from Figure 16e and the average recovery from Table 3 for the sample analyzed on 04-Dec-2001:

$$5\text{-OH conc.} \quad = \quad \frac{5\text{-OH conc.}}{\text{(gross ng/g)}} \times \left(\frac{100}{\text{Average \% recovery}} \right)$$

$$5\text{-OH conc.} \quad = \quad 2.74 \text{ ng/g} \times \frac{100}{95}$$

$$5\text{-OH conc.} \quad = \quad 2.88 \text{ ng/g}$$

10.7. Determination of Soil Moisture

- 10.7.1. Accurately weigh a 10-g portion of soil into a tarred aluminum weighing dish.
- 10.7.2. Place the sample in an oven at 110 °C and allow to dry for a minimum of 16 hours.
- 10.7.3. Remove the sample from the oven and place in a dessicator containing Drierite adsorbent. Re-weigh the sample when it has cooled to room temperature.
- 10.7.4. Calculate the percent moisture (dry weight basis) as follows:

$$\text{Percent Moisture} \quad = \quad \frac{\text{water, g}}{\text{dry soil, g}} \times 100$$

$$\text{Percent Moisture} \quad = \quad \frac{\left(\text{sample weight before drying, g} \right) - \left(\text{sample weight after drying, g} \right)}{\text{sample weight after drying, g}} \times 100$$

10.8. Determination of Dry Weight Concentrations of XDE-638 and Metabolites in Sediment and Soil

- 10.8.1. Determine the analyte concentrations in the sample as described in Sections 10.3. and 10.6.
- 10.8.2. Determine the soil moisture as described in Section 10.7.
- 10.8.3. Determine the dry weight analyte concentrations in the samples as follows:

$$\text{XDE-638 Conc. (dry weight ng/g)} = \text{XDE-638 Conc. (ng/g)} \times \left(1 + \frac{\% \text{ Moisture}}{100}\right)$$

11. RESULTS AND DISCUSSION

11.1. Method Validation

11.1.1. Recovery Levels and Precision

A method validation study was conducted to determine the recovery levels and the precision of the method for the determination of XDE-638 and metabolites in soil and sediment. The results are summarized below and listed individually in Tables 2-7.

Compound	Matrix	Average Recovery %	Standard Deviation %
XDE-638	Soil/Sediment	84	5.4
5-OH Metabolite	Soil/Sediment	95	4.6
Sulfonamide Metabolite	Soil/Sediment	86	6.2
BSTCA Metabolite	Soil/Sediment	86	4.4
BSA Metabolite	Soil/Sediment	94	6.3
2-Amino-TP Metabolite	Soil/Sediment	97	10.2

For XDE-638 and metabolites analysis, all of the individual recovery samples in the case of each of the analytes were between 70 and 120% with standard deviations less than 20%.

11.1.2. Standard Curve Linearity

For the linear regression analysis, the correlation coefficients (*r*) were greater than 0.999 for each of the analytes for all of the calibration curve determinations during the method validation. The results indicate linearity of the detector response as a function of the standard calibration curve.

11.1.3. Calculated Limits of Quantitation and Detection

Following established guidelines (13.2), the limits of quantitation (LOQ) and detection (LOD) were calculated for all six analytes using the standard deviation from the 3-nug/g recovery results. The LOQ was calculated as ten times the standard deviation ($10s$), and the LOD was calculated as three times the standard deviation ($3s$) of the results of the analysis of 12 samples for each analyte. The results are summarized below and individual values are presented in Tables 2-7.

Compound	Matrix	Average Recovery ng/g	Standard Deviation (s)	Limit of Detection ($3s$)	Limit of Quantitation ($10s$)
XDE-638	Soil/Sediment	2.53	0.19	0.58	1.94
5-OH	Soil/Sediment	2.92	0.22	0.67	2.23
Sulfonamide	Soil/Sediment	2.77	0.19	0.56	1.87
BSTCA	Soil/Sediment	2.62	0.18	0.53	1.77
BSA	Soil/Sediment	2.98	0.18	0.53	1.78
2-Amino-TP	Soil/Sediment	2.94	0.34	1.01	3.36

The calculated LOQ supported the validated LOQ of 3.0 ng/g for all analytes. Since the lowest level of fortification for recovery samples was 3.0 ng/g for each analyte, the method LOQ is considered to be 3.0 ng/g.

Similarly, the calculated LOD for all analytes ranged from 0.53 to 1.01 ng/g for all analytes.

11.2. Confirmation of Residue Identity

The presence of XDE-638 and metabolites is confirmed by comparing the liquid chromatography retention times of the analytes in the calibration standards with those found in the samples as well as by the MS/MS transitions monitored. Due to the highly specific nature of the MS/MS transitions monitored during detection, no further confirmation technique is required.

11.3. Assay Time and Stopping Points

A typical analytical run would consist of a minimum of eight standards encompassing the expected range of sample concentrations, a reagent blank, a control (a non-fortified sample), a minimum of three fortified controls (two of which must be at the LOQ), and 19 samples. This typical analytical set can be prepared in approximately 4 hours followed by the chromatographic analysis.

There are no acceptable stopping points during sample extraction and cleanup due to the instability of some of the metabolites. Samples can be stored overnight in a refrigerator at step 9.3.13 with no significant loss in analyte recovery.

11.4. Standardization of HLB SPE Elution Profile

- 11.4.1. Add 100 μ L of a 1.0- μ g/mL mixed standard (Section 7.2.8) into 10.0 mL of 0.1 N hydrochloric acid.
 - a. Condition a Waters HLB 96-well plate (30-mg) with 0.2 mL of methanol followed by 1.0 mL 0.1 N hydrochloric acid (dry the plate at full vacuum for 10 seconds between solvents.)
 - b. Transfer 1.50 mL of the sample solution from Step 11.4.1 to the 96-well plate. Draw the sample through the plate at approximately 1 mL/min collecting the eluate in a deep well collection rack. Dry the plate at full vacuum for 10 seconds after sample has eluted.
 - c. Wash the plate with 1 mL of water:methanol (95: 5 v/v) solution, collecting the eluate in a deep well collection rack. Dry the plate at full vacuum for 10 seconds after the sample has all passed through the plate.
 - d. Elute the XDE-638 and metabolites from the plate at approximately 1 mL/min with three 1.0-mL aliquots of acetonitrile:methanol (80:20), collecting the eluate in separate 2-mL deep-well racks.
- 11.4.2. Using a transfer pipet, transfer the three 1.0-mL aliquots of acetonitrile:methanol (80:20) to a clean 40-mL vials and evaporate to dryness using a TurboVap evaporator set at 40°C and a nitrogen pressure of 10 psi.
- 11.4.3. Reconstitute the samples from Step 11.4.2. in 1.0 mL of 0.005- μ g/mL XDE-638 stable-isotope internal standard in methanol:acetonitrile:water:acetic acid (5:5:90:0.1). Sonicate and vortex mix the sample vials for approximately 30 seconds.
- 11.4.4. Transfer the samples from Sections 11.4.1 b, 11.4.1.c and 11.4.3 to a 2-mL autosampler vial, and seal the vial with a cap. Analyze the samples along with the calibration standards. Calculate the percent recovery as described in Section 10.

Typical elution profiles are illustrated in Figure 18. If the elution profiles differ from those shown, adjust the volume of acetonitrile:methanol (80:20 v/v) to be collected in Step 9.3.13.d.

12. NOTES

- 12.1. Equipment, glassware, materials, reagents, and chemicals considered to be equivalent to those specified may be substituted with the understanding that their performance must be confirmed by appropriate tests. Common laboratory supplies are assumed to be readily available and are, therefore, not listed.

- 12.2. Section 7 provides suggested concentrations for calibration standard preparation. Other dilution schemes may be followed.
 - 12.3. The data presented in this method was generated using a Sciex 3000 API 3000 in optimal condition. Operating conditions may be modified to obtain optimal separation or sensitivity. However, method performance will be compromised by increasing injection volume to compensate for low instrument sensitivity.
 - 12.4. Before using each lot of HLB SPE Plates, determine the elution profile as described in section 11.4.
 - 12.5. Linear Regression analysis using $1/x$ weighting or quadratic curve fit may also be used.
13. REFERENCES
- 13.1. Freund, J. E.; Williams, F. J. *Dictionary/Outline of Basic Statistics*; Dover: New York, 1991; p 170.
 - 13.2. Keith, L. H.; Crummett, W.; Deegan, J., Jr.; Libby, R. A.; Taylor, J. K.; Wentler, G. *Anal. Chem.* 1983, 55, 2210-2218.

The information herein is presented in good faith, but no warranty, express or implied, is given nor is freedom from any patent owned by Dow AgroSciences LLC or by others to be inferred. In the hands of qualified personnel, the procedures are expected to yield results of sufficient accuracy for their intended purposes, but recipients are cautioned to confirm the reliability of their techniques, equipment, and standards by appropriate tests. Anyone wishing to reproduce or publish the material in whole or in part should request written permission from Dow AgroSciences LLC.

Table 1. Chemical Names and Structures for XDE-638, Metabolites, and Internal Standards

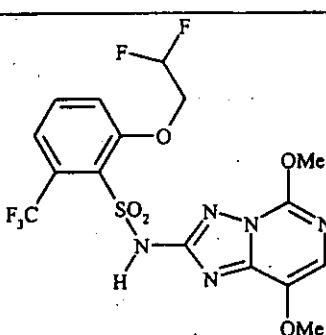
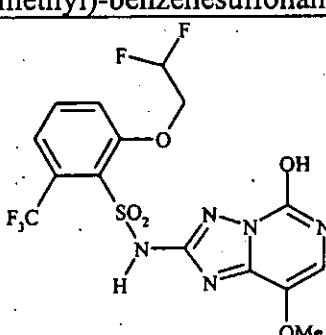

Common Name of Compound	Structure and CAS Name
XDE-638 Molecular Formula: C ₁₆ H ₁₄ F ₅ N ₅ O ₅ S Molecular Weight: 483 CAS Number: 219714-96-2	 2-(2,2-difluoroethoxy)-N-(5,8-dimethoxy[1,2,4]triazolo[1,5-c]pyrimidin-2-yl)-6-(trifluoromethyl)-benzenesulfonamide
5-OH Metabolite of XDE-638 Molecular Formula: C ₁₅ H ₁₂ F ₅ N ₅ O ₅ S Molecular Weight: 469 CAS Number: NA	 2-(2,2-difluoroethoxy)-N-(5,6-dihydro-8-methoxy-5-oxo[1,2,4]triazolo[1,5-c]pyrimidin-2-yl)-6-(trifluoromethyl)-benzenesulfonamide
Sulfonamide Metabolite of XDE-638 Molecular Formula: C ₉ H ₈ F ₅ NO ₃ S Molecular Weight: 305 CAS Number: NA	 2-(2,2-difluoroethoxy)-6-(trifluoromethyl)-benzenesulfonamide

Table 1. (Cont.) Chemical Names and Structures for XDE-638, Metabolites, and Internal Standard

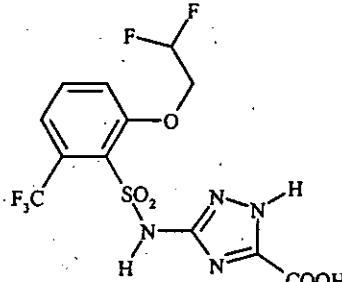


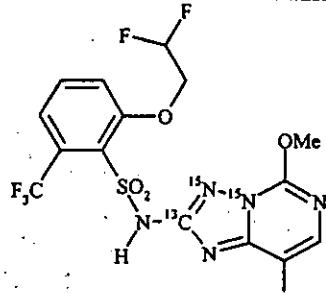
Common Name of Compound	Structure and CAS Name
BSTCA Metabolite of XDE-638	 <p>5-[[[2-(2,2-difluoroethoxy)-6-(trifluoromethyl) phenyl]sulfonyl]amino]-1<i>H</i>-1,2,4-triazole-3-carboxylic acid</p>
BSA Metabolite of XDE-638	 <p>2-(2,2-Difluoroethoxy)-6-(trifluoromethyl) benzenesulfonic acid</p>
2-Amino-TP Metabolite of XDE-638	 <p>5,8-Dimethoxy[1,2,4]triazolo[1,5-<i>c</i>]pyrimidin-2-amine</p>
M+3 Stable Isotope of XDE-638	 <p>2-(2,2-difluoroethoxy)-<i>N</i>-(5,8-dimethoxy[1,2,4]triazolo[1,5-<i>c</i>]pyrimidin-2-yl-2-¹³C-3,4-¹⁵N2)-6-(trifluoromethyl) benzenesulfonamide</p>

Table 2. Recovery of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	XDE-638, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.105	--	
SN36984501	04-Mar-2002	1.00	0.89	N/A	
SN32982701	04-Mar-2002	1.00	0.56	N/A	
SN34120701	04-Mar-2002	1.00	0.65	N/A	
SN36984501	03-Dec-2001	3.00	2.58	86	
SN36984501	03-Dec-2001	3.00	2.54	85	
SN32982701	03-Dec-2001	3.00	2.23	74	
SN32982701	03-Dec-2001	3.00	2.62	87	
SN34120701	03-Dec-2001	3.00	2.39	80	
SN34120701	03-Dec-2001	3.00	2.95	98	
SN34120701	04-Dec-2001	3.00	2.53	84	
SN34120701	04-Dec-2001	3.00	2.65	88	$\bar{x} = 2.53$
SN32982701	04-Dec-2001	3.00	2.56	85	$s = 0.19$
SN32982701	04-Dec-2001	3.00	2.58	86	$3s^b = 0.58$
SN36984501	04-Dec-2001	3.00	2.46	82	$10s^c = 1.94$
SN36984501	04-Dec-2001	3.00	2.22	74	
		Average	84		
		SD	6.4		
		RSD	7.6		
		n	12		
SN36984501	03-Dec-2001	10.0	8.68	87	
SN36984501	03-Dec-2001	10.0	8.29	83	
SN32982701	03-Dec-2001	10.0	8.65	87	
SN32982701	03-Dec-2001	10.0	7.92	79	$\bar{x} = 8.39$
SN34120701	04-Dec-2001	10.0	8.37	84	$s = 0.28$
SN34120701	04-Dec-2001	10.0	8.43	84	
		Average	84		
		SD	2.8		
		RSD	3.3		
		n	6		

Table 2. (Cont.) Recovery of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	XDE-638, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	41.98	84	
SN36984501	03-Dec-2001	50.0	43.42	87	
SN32982701	03-Dec-2001	50.0	36.11	72	
SN32982701	03-Dec-2001	50.0	43.28	87	$\bar{x} = 41.30$
SN34120701	04-Dec-2001	50.0	41.41	83	$s = 2.68$
SN34120701	04-Dec-2001	50.0	41.59	83	
		Average		83	
		SD		5.4	
		RSD		6.5	
		n		6	
SN36984501	03-Dec-2001	100.0	72.24	72	
SN36984501	03-Dec-2001	100.0	74.89	75	
SN32982701	03-Dec-2001	100.0	84.24	84	
SN32982701	03-Dec-2001	100.0	83.98	84	$\bar{x} = 81.12$
SN34120701	04-Dec-2001	100.0	85.63	86	$s = 5.96$
SN34120701	04-Dec-2001	100.0	85.75	86	
		Average		81	
		SD		6.0	
		RSD		7.4	
		n		6	
		Overall Average		84	
		Overall SD		5.4	
		Overall RSD		6.5	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

Table 3. Recovery of 5-OH Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	5-OH, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.000	--	
SN36984501	04-Mar-2002	1.00	0.98	N/A	
SN32982701	04-Mar-2002	1.00	1.29	N/A	
SN34120701	04-Mar-2002	1.00	1.15	N/A	
SN36984501	03-Dec-2001	3.00	2.74	91	
SN36984501	03-Dec-2001	3.00	2.65	88	
SN32982701	03-Dec-2001	3.00	2.97	99	
SN32982701	03-Dec-2001	3.00	3.04	101	
SN34120701	03-Dec-2001	3.00	3.04	101	
SN34120701	03-Dec-2001	3.00	3.10	103	
SN34120701	04-Dec-2001	3.00	2.66	89	
SN34120701	04-Dec-2001	3.00	2.84	95	$\bar{x} = 2.92$
SN32982701	04-Dec-2001	3.00	2.82	94	$s = 0.22$
SN32982701	04-Dec-2001	3.00	2.93	98	$3s^b = 0.67$
SN36984501	04-Dec-2001	3.00	2.76	92	$10s^c = 2.23$
SN36984501	04-Dec-2001	3.00	3.44	115	
		Average	97		
		SD	7.5		
		RSD	7.7		
		n	12		
SN36984501	03-Dec-2001	10.0	9.12	91	
SN36984501	03-Dec-2001	10.0	9.41	94	
SN32982701	03-Dec-2001	10.0	9.40	94	
SN32982701	03-Dec-2001	10.0	9.89	99	$\bar{x} = 9.39$
SN34120701	04-Dec-2001	10.0	9.40	94	$s = 0.28$
SN34120701	04-Dec-2001	10.0	9.14	91	
		Average	94		
		SD	2.8		
		RSD	3.0		
		n	6		

Table 3. (Cont.) Recovery of 5-OH Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	5-OH, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	45.74	92	
SN36984501	03-Dec-2001	50.0	45.10	90	
SN32982701	03-Dec-2001	50.0	48.67	97	
SN32982701	03-Dec-2001	50.0	45.76	92	$\bar{x} = 46.70$
SN34120701	04-Dec-2001	50.0	48.65	97	$s = 1.56$
SN34120701	04-Dec-2001	50.0	46.27	93	
		Average		93	
		SD		3.1	
		RSD		3.3	
		n		6	
SN36984501	03-Dec-2001	100.0	101.58	102	
SN36984501	03-Dec-2001	100.0	99.66	100	
SN32982701	03-Dec-2001	100.0	88.37	88	
SN32982701	03-Dec-2001	100.0	90.99	91	$\bar{x} = 93.80$
SN34120701	04-Dec-2001	100.0	91.97	92	$s = 5.45$
SN34120701	04-Dec-2001	100.0	90.24	90	
		Average		94	
		SD		5.5	
		RSD		5.8	
		n		6	
		Overall Average		95	
		Overall SD		4.6	
		Overall RSD		4.8	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

Table 4. Recovery of Sulfonamide Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	Sulfonamide, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.115	--	
SN36984501	04-Mar-2002	1.00	0.81	N/A	
SN32982701	04-Mar-2002	1.00	0.92	N/A	
SN34120701	04-Mar-2002	1.00	0.84	N/A	
SN36984501	03-Dec-2001	3.00	2.47	83	
SN36984501	03-Dec-2001	3.00	2.49	83	
SN32982701	03-Dec-2001	3.00	2.57	86	
SN32982701	03-Dec-2001	3.00	2.79	93	
SN34120701	03-Dec-2001	3.00	2.81	94	
SN34120701	03-Dec-2001	3.00	2.71	90	
SN34120701	04-Dec-2001	3.00	2.69	90	
SN34120701	04-Dec-2001	3.00	2.95	98	$\bar{x} = 2.77$
SN32982701	04-Dec-2001	3.00	3.00	100	$s = 0.19$
SN32982701	04-Dec-2001	3.00	2.97	99	$3s^b = 0.56$
SN36984501	04-Dec-2001	3.00	2.85	95	$10s^c = 1.87$
SN36984501	04-Dec-2001	3.00	2.95	98	
		Average	93		
		SD	6.2		
		RSD	6.7		
		n	12		
SN36984501	03-Dec-2001	10.0	7.60	76	
SN36984501	03-Dec-2001	10.0	8.20	82	
SN32982701	03-Dec-2001	10.0	8.54	85	
SN32982701	03-Dec-2001	10.0	7.86	79	$\bar{x} = 8.40$
SN34120701	04-Dec-2001	10.0	9.50	95	$s = 0.68$
SN34120701	04-Dec-2001	10.0	8.72	87	
		Average	84		
		SD	6.8		
		RSD	8.1		
		n	6		

Table 4. (Cont.) Recovery of Sulfonamide Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	Sulfonamide, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	39.16	78	
SN36984501	03-Dec-2001	50.0	38.07	76	
SN32982701	03-Dec-2001	50.0	39.16	78	
SN32982701	03-Dec-2001	50.0	39.00	78	$\bar{x} = 40.66$
SN34120701	04-Dec-2001	50.0	43.61	87	$s = 2.86$
SN34120701	04-Dec-2001	50.0	44.94	90	
		Average		81	
		SD		5.7	
		RSD		7.1	
		n		6	
SN36984501	03-Dec-2001	100.0	75.07	75	
SN36984501	03-Dec-2001	100.0	75.73	76	
SN32982701	03-Dec-2001	100.0	77.69	78	
SN32982701	03-Dec-2001	100.0	78.05	78	$\bar{x} = 79.69$
SN34120701	04-Dec-2001	100.0	87.18	87	$s = 4.95$
SN34120701	04-Dec-2001	100.0	84.43	84	
		Average		80	
		SD		5.0	
		RSD		6.3	
		n			
		Overall Average		86	
		Overall SD		6.2	
		Overall RSD		7.2	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

Table 5. Recovery of BSTCA Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	BSTCA, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.09	--	
SN36984501	04-Mar-2002	1.00	0.83	N/A	
SN32982701	04-Mar-2002	1.00	0.95	N/A	
SN34120701	04-Mar-2002	1.00	0.83	N/A	
SN36984501	03-Dec-2001	3.00	2.37	79	
SN36984501	03-Dec-2001	3.00	2.38	79	
SN32982701	03-Dec-2001	3.00	2.59	86	
SN32982701	03-Dec-2001	3.00	2.63	88	
SN34120701	03-Dec-2001	3.00	2.75	92	
SN34120701	03-Dec-2001	3.00	2.74	91	
SN34120701	04-Dec-2001	3.00	2.47	82	
SN34120701	04-Dec-2001	3.00	2.40	80	$\bar{x} = 2.62$
SN32982701	04-Dec-2001	3.00	2.74	91	$s = 0.18$
SN32982701	04-Dec-2001	3.00	2.77	92	$3s^b = 0.53$
SN36984501	04-Dec-2001	3.00	2.64	88	$10s^c = 1.77$
SN36984501	04-Dec-2001	3.00	2.91	97	
		Average	88		
		SD	5.9		
		RSD	6.7		
		n	12		
SN36984501	03-Dec-2001	10.0	9.06	91	
SN36984501	03-Dec-2001	10.0	8.82	88	
SN32982701	03-Dec-2001	10.0	7.99	80	
SN32982701	03-Dec-2001	10.0	8.58	86	$\bar{x} = 8.51$
SN34120701	04-Dec-2001	10.0	8.39	84	$s = 0.39$
SN34120701	04-Dec-2001	10.0	8.21	82	
		Average	85		
		SD	3.9		
		RSD	4.6		
		n	6		

Table 5. (Cont.) Recovery of BSTCA Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	BSTCA, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	42.20	84	
SN36984501	03-Dec-2001	50.0	42.19	84	
SN32982701	03-Dec-2001	50.0	40.76	82	
SN32982701	03-Dec-2001	50.0	41.89	84	$\bar{x} = 42.05$
SN34120701	04-Dec-2001	50.0	43.89	88	$s = 1.06$
SN34120701	04-Dec-2001	50.0	41.34	83	
		Average		84	
		SD		2.1	
		RSD		2.5	
		n		6	
SN36984501	03-Dec-2001	100.0	86.33	86	
SN36984501	03-Dec-2001	100.0	86.15	86	
SN32982701	03-Dec-2001	100.0	81.74	82	
SN32982701	03-Dec-2001	100.0	83.60	84	$\bar{x} = 84.32$
SN34120701	04-Dec-2001	100.0	87.46	88	$s = 2.76$
SN34120701	04-Dec-2001	100.0	80.61	81	
		Average		84	
		SD		2.8	
		RSD		3.3	
		n		6	
		Overall Average		86	
		Overall SD		4.4	
		Overall RSD		5.2	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

Table 6. Recovery of BSA Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	BSA, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.105	--	
SN36984501	04-Mar-2002	1.00	0.94	N/A	
SN32982701	04-Mar-2002	1.00	1.08	N/A	
SN34120701	04-Mar-2002	1.00	0.95	N/A	
SN36984501	03-Dec-2001	3.00	2.68	89	
SN36984501	03-Dec-2001	3.00	2.74	91	
SN32982701	03-Dec-2001	3.00	2.99	100	
SN32982701	03-Dec-2001	3.00	2.97	99	
SN34120701	03-Dec-2001	3.00	2.92	97	
SN34120701	03-Dec-2001	3.00	3.10	104	
SN34120701	04-Dec-2001	3.00	2.91	97	
SN34120701	04-Dec-2001	3.00	3.06	102	$\bar{x} = 2.98$
SN32982701	04-Dec-2001	3.00	2.95	98	$s = 0.18$
SN32982701	04-Dec-2001	3.00	3.12	104	$3s^b = 0.53$
SN36984501	04-Dec-2001	3.00	2.99	100	$10s^c = 1.78$
SN36984501	04-Dec-2001	3.00	3.37	112	
		Average	99		
		SD	5.9		
		RSD	6.0		
		n	12		
SN36984501	03-Dec-2001	10.0	9.22	92	
SN36984501	03-Dec-2001	10.0	9.47	95	
SN32982701	03-Dec-2001	10.0	9.40	94	
SN32982701	03-Dec-2001	10.0	9.43	94	$\bar{x} = 9.48$
SN34120701	04-Dec-2001	10.0	10.23	102	$s = 0.11$
SN34120701	04-Dec-2001	10.0	9.15	92	
		Average	95		
		SD	3.9		
		RSD	4.1		
		n	6		

Table 6. (Cont.) Recovery of BSA Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	BSA, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	44.70	89	
SN36984501	03-Dec-2001	50.0	43.20	86	
SN32982701	03-Dec-2001	50.0	45.54	91	
SN32982701	03-Dec-2001	50.0	44.39	89	$\bar{x} = 45.15$
SN34120701	04-Dec-2001	50.0	47.25	95	$s = 1.38$
SN34120701	04-Dec-2001	50.0	45.80	92	
		Average		90	
		SD		2.8	
		RSD		3.1	
		n		6	
SN36984501	03-Dec-2001	100.0	85.51	86	
SN36984501	03-Dec-2001	100.0	88.43	88	
SN32982701	03-Dec-2001	100.0	86.89	87	
SN32982701	03-Dec-2001	100.0	88.75	89	$\bar{x} = 88.23$
SN34120701	04-Dec-2001	100.0	90.98	91	$s = 1.87$
SN34120701	04-Dec-2001	100.0	88.81	89	
		Average		88	
		SD		1.9	
		RSD		2.1	
		n		6	
		Overall Average		94	
		Overall SD		6.3	
		Overall RSD		6.7	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

Table 7. Recovery of 2-Amino-TP Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	2-Amino-TP, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	0.000	0.000	--	
SN32982701	03-Dec-2001	0.000	0.000	--	
SN34120701	04-Dec-2001	0.000	0.14	--	
SN36984501	04-Mar-2002	1.00	0.73	N/A	
SN32982701	04-Mar-2002	1.00	0.93	N/A	
SN34120701	04-Mar-2002	1.00	0.90	N/A	
SN36984501	03-Dec-2001	3.00	2.51	84	
SN36984501	03-Dec-2001	3.00	2.45	82	
SN32982701	03-Dec-2001	3.00	2.98	99	
SN32982701	03-Dec-2001	3.00	3.39	113	
SN34120701	03-Dec-2001	3.00	3.20	107	
SN34120701	03-Dec-2001	3.00	2.97	99	
SN34120701	04-Dec-2001	3.00	2.74	91	
SN34120701	04-Dec-2001	3.00	2.95	99	$\bar{x} = 2.94$
SN32982701	04-Dec-2001	3.00	3.19	106	$s = 0.34$
SN32982701	04-Dec-2001	3.00	3.46	115	$3s^b = 1.01$
SN36984501	04-Dec-2001	3.00	2.53	84	$10s^c = 3.36$
SN36984501	04-Dec-2001	3.00	2.94	98	
		Average	98		
		SD	11.2		
		RSD	11.4		
		n	12		
SN36984501	03-Dec-2001	10.0	8.57	86	
SN36984501	03-Dec-2001	10.0	9.95	100	
SN32982701	03-Dec-2001	10.0	9.53	95	
SN32982701	03-Dec-2001	10.0	10.51	105	$\bar{x} = 9.82$
SN34120701	04-Dec-2001	10.0	10.76	108	$s = 0.78$
SN34120701	04-Dec-2001	10.0	9.59	96	
		Average	99		
		SD	7.8		
		RSD	8.0		
		n	6		

Table 7. (Cont.) Recovery of 2-Amino-TP Metabolite of XDE-638 from Soil and Sediment

Sample Number	Date of Analysis	2-Amino-TP, ng/g		Recovery ^a %	Statistical Calculations, ng/g
		Added	Found		
SN36984501	03-Dec-2001	50.0	40.53	81	
SN36984501	03-Dec-2001	50.0	40.38	81	
SN32982701	03-Dec-2001	50.0	48.00	96	
SN32982701	03-Dec-2001	50.0	48.34	97	$\bar{x} = 46.38$
SN34120701	04-Dec-2001	50.0	52.27	105	$s = 4.84$
SN34120701	04-Dec-2001	50.0	48.73	98	
		Average		93	
		SD		9.6	
		RSD		10.4	
		n		6	
SN36984501	03-Dec-2001	100.0	80.54	81	
SN36984501	03-Dec-2001	100.0	83.81	84	
SN32982701	03-Dec-2001	100.0	103.25	103	
SN32982701	03-Dec-2001	100.0	106.85	107	$\bar{x} = 95.82$
SN34120701	04-Dec-2001	100.0	108.79	109	$s = 12.17$
SN34120701	04-Dec-2001	100.0	91.68	92	
		Average		96	
		SD		12.2	
		RSD		12.7	
		n		6	
		Overall Average		97	
		Overall SD		10.2	
		Overall RSD		10.6	
		Overall n		30	

^a All calculations were performed in Microsoft Excel 97 with full precision.

^b Calculated limit of detection.

^c Calculated limit of quantitation.

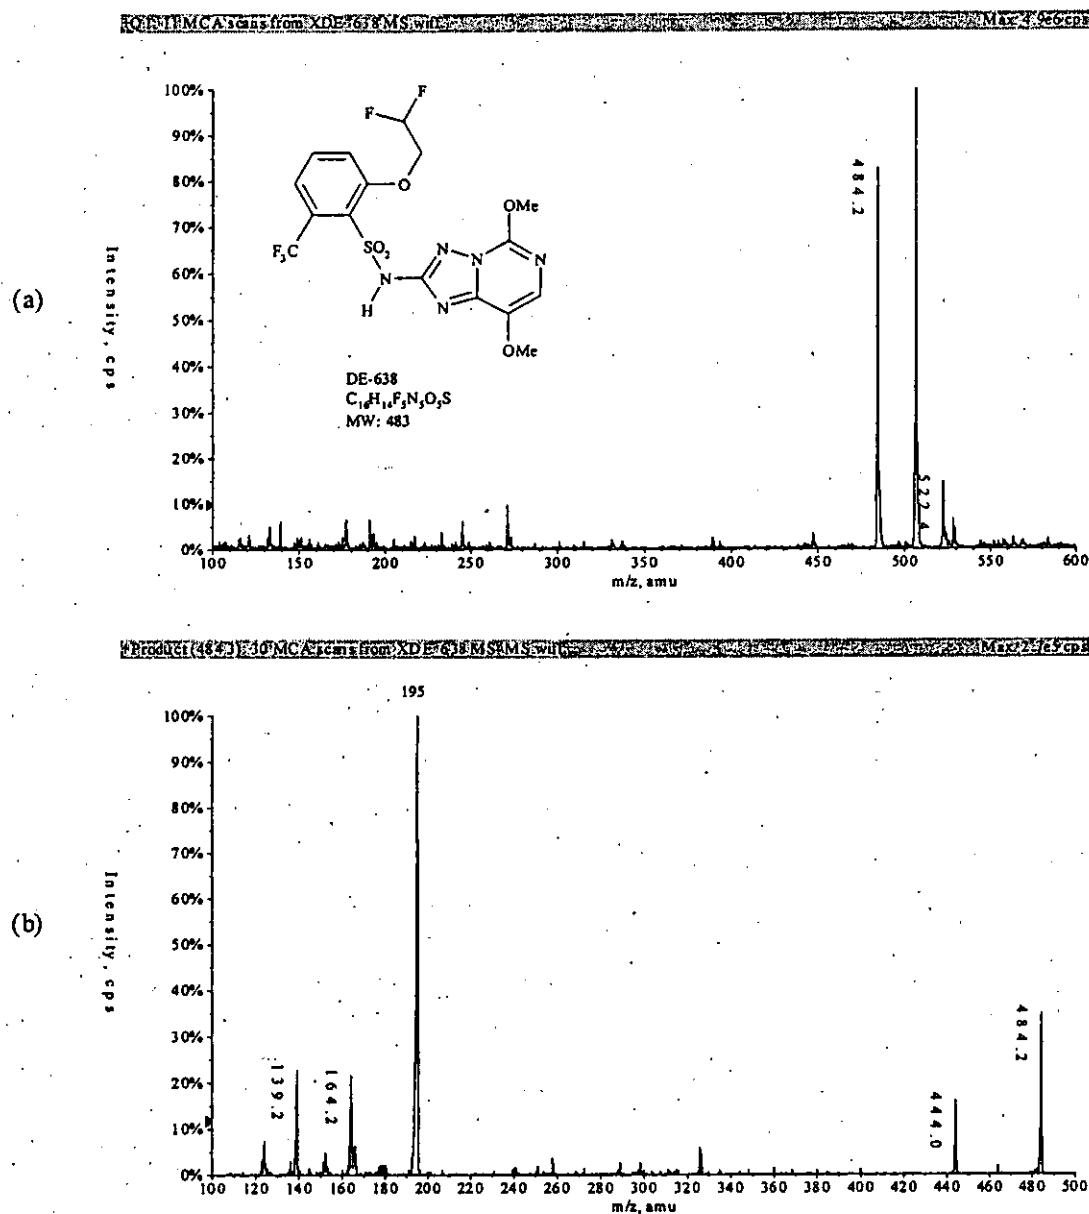


Figure 1. Mass Spectra for XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Positive Ionization ($M+H$)⁺ at m/z 484 (b) Product-Ion Mass Spectrum of XDE-638 Showing Fragment Ion at m/z 195

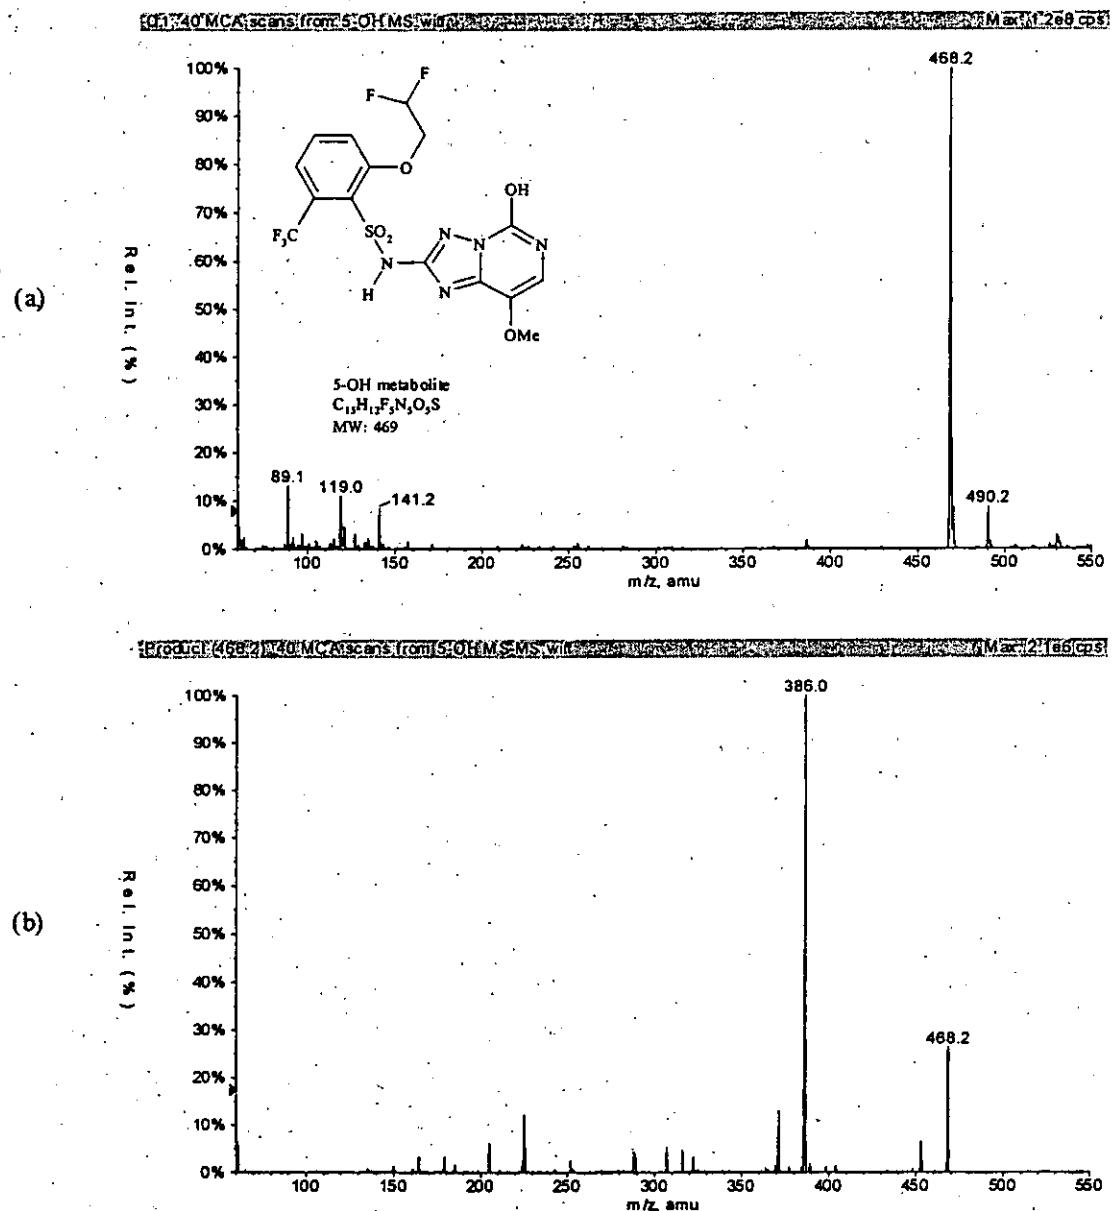


Figure 2. Mass Spectra for 5-OH XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Negative Ionization ($M-H^-$) at m/z 468 (b) Product-Ion Mass Spectrum of 5-OH XDE-638 Showing Fragment Ion at m/z 386

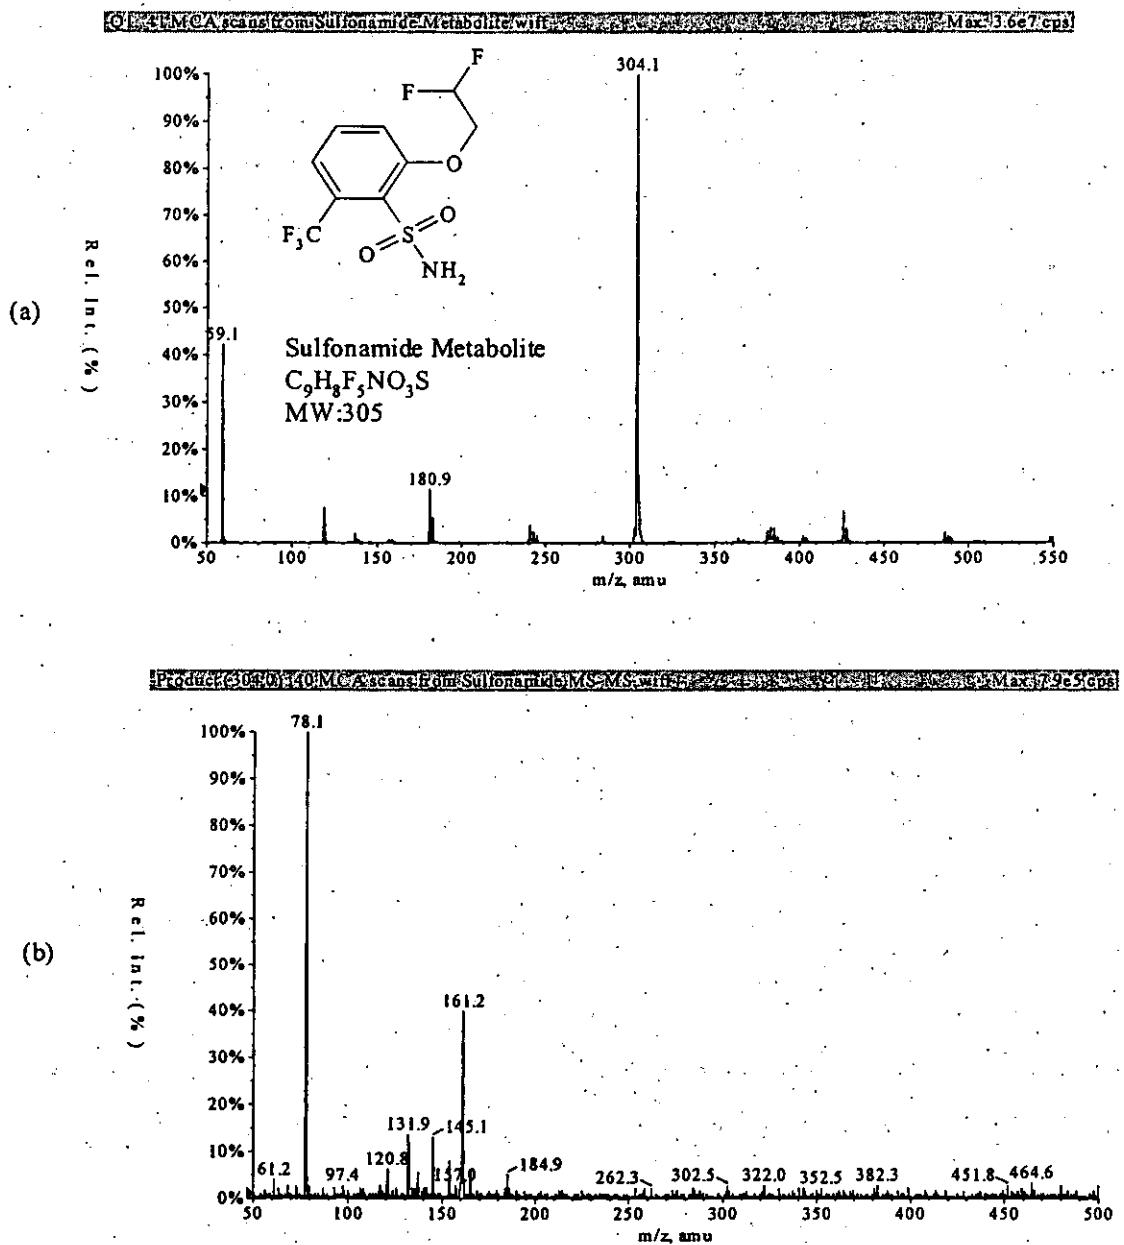


Figure 3. Mass Spectra for Sulfonamide Metabolite of XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Negative Ionization ($M-H^-$) at m/z 304 (b) Product-Ion Mass Spectrum of the Sulfonamide Metabolite of XDE-638 Showing Fragment Ion at m/z 78

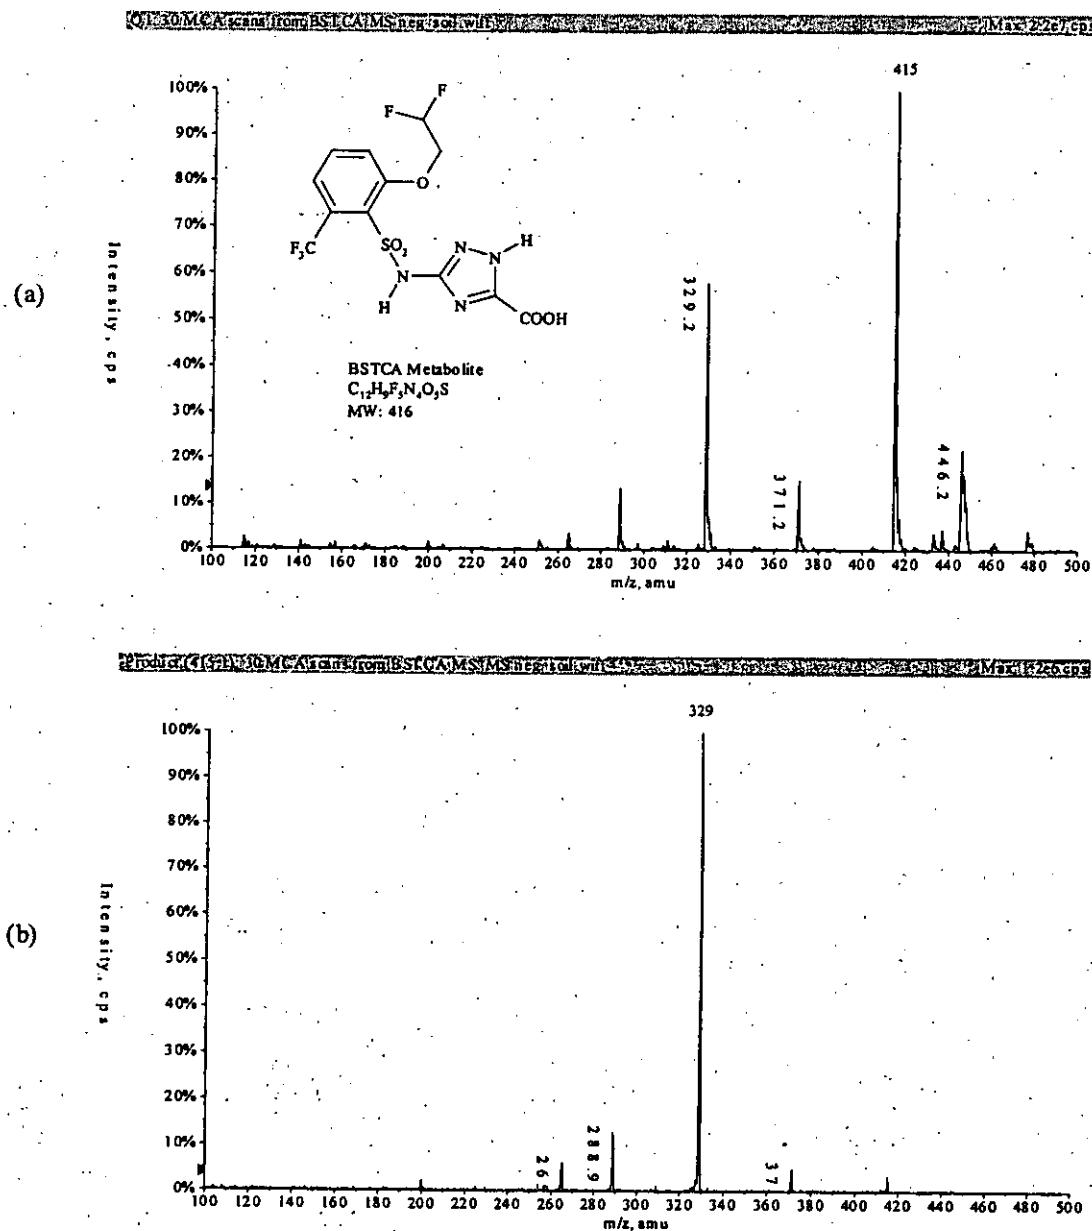


Figure 4. Mass Spectra for BSTCA of XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Negative Ionization ($M-H^-$) at m/z 415 (b) Product-Ion Mass Spectrum of the BSTCA Metabolite of XDE-638 Showing Fragment Ion at m/z 329

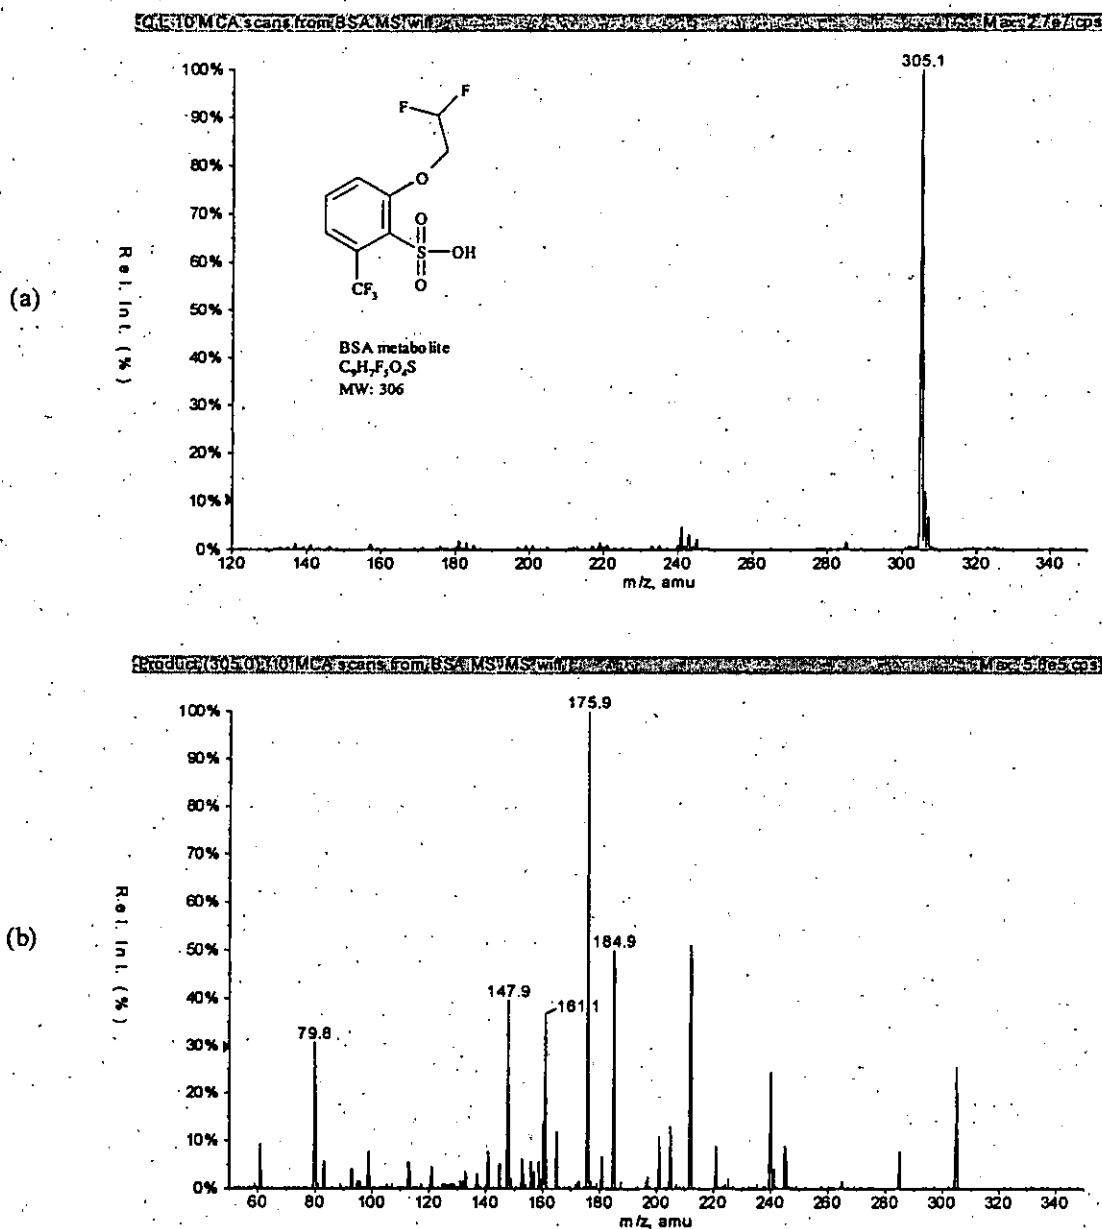


Figure 5. Mass Spectra for BSA of XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Negative Ionization ($M-H^-$) at m/z 305 (b) Product-Ion Mass Spectrum of the BSTCA Metabolite of XDE-638 Showing Fragment Ion at m/z 176

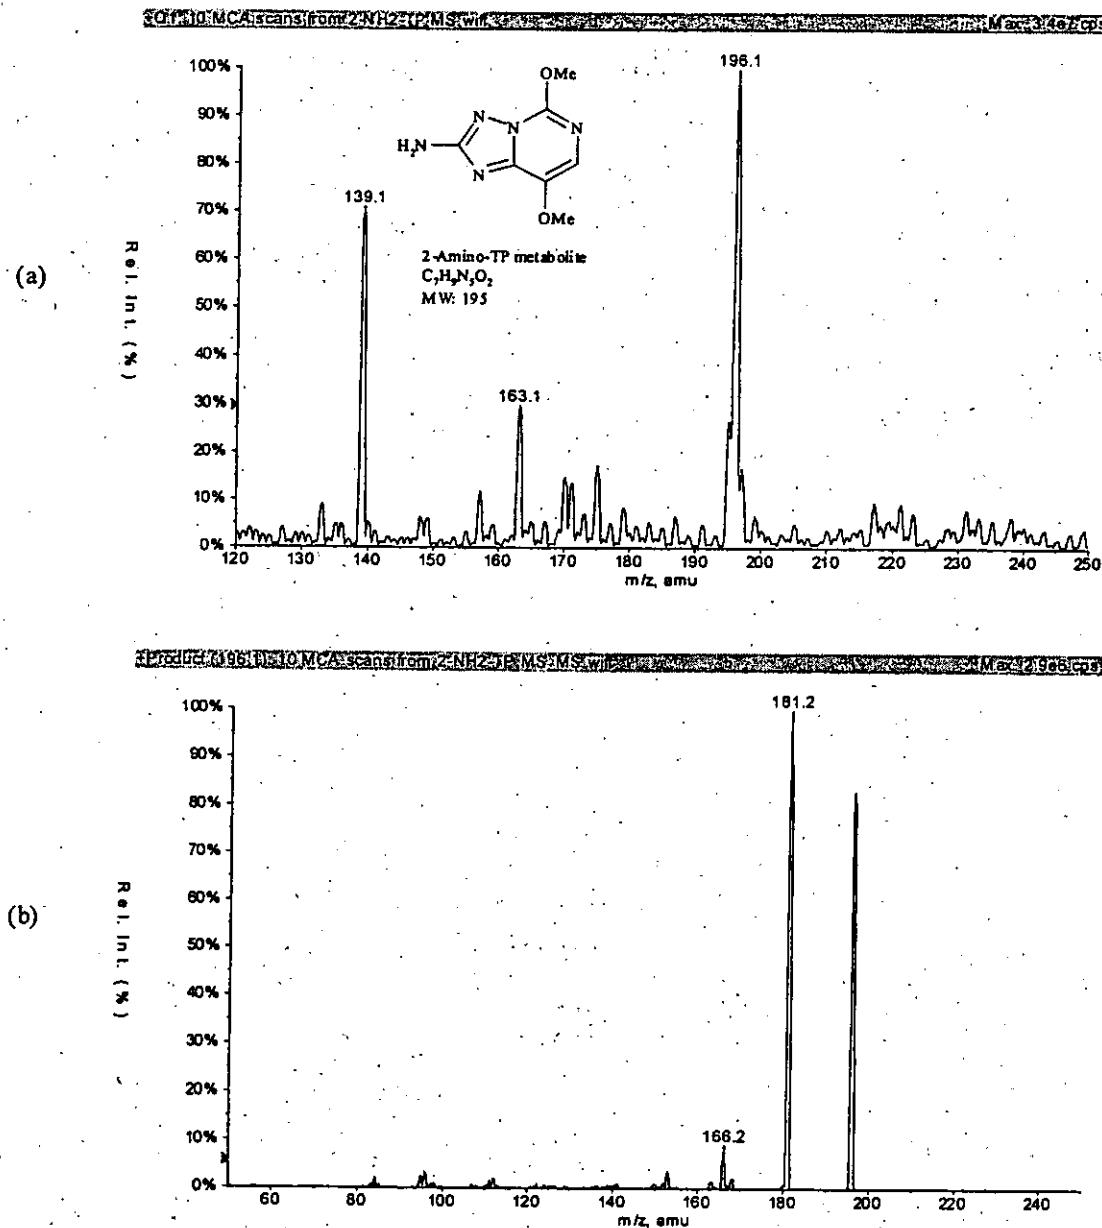


Figure 6. Mass Spectra for 2-Amino-TP Metabolite of XDE-638: (a) Mass Spectrum for Q1 Scan using Electrospray Positive Ionization ($M+H$)⁺ at m/z 196 (b) Product-Ion Mass Spectrum of the 2-Amino-TP Metabolite of XDE-638 Showing Fragment Ion at m/z 181


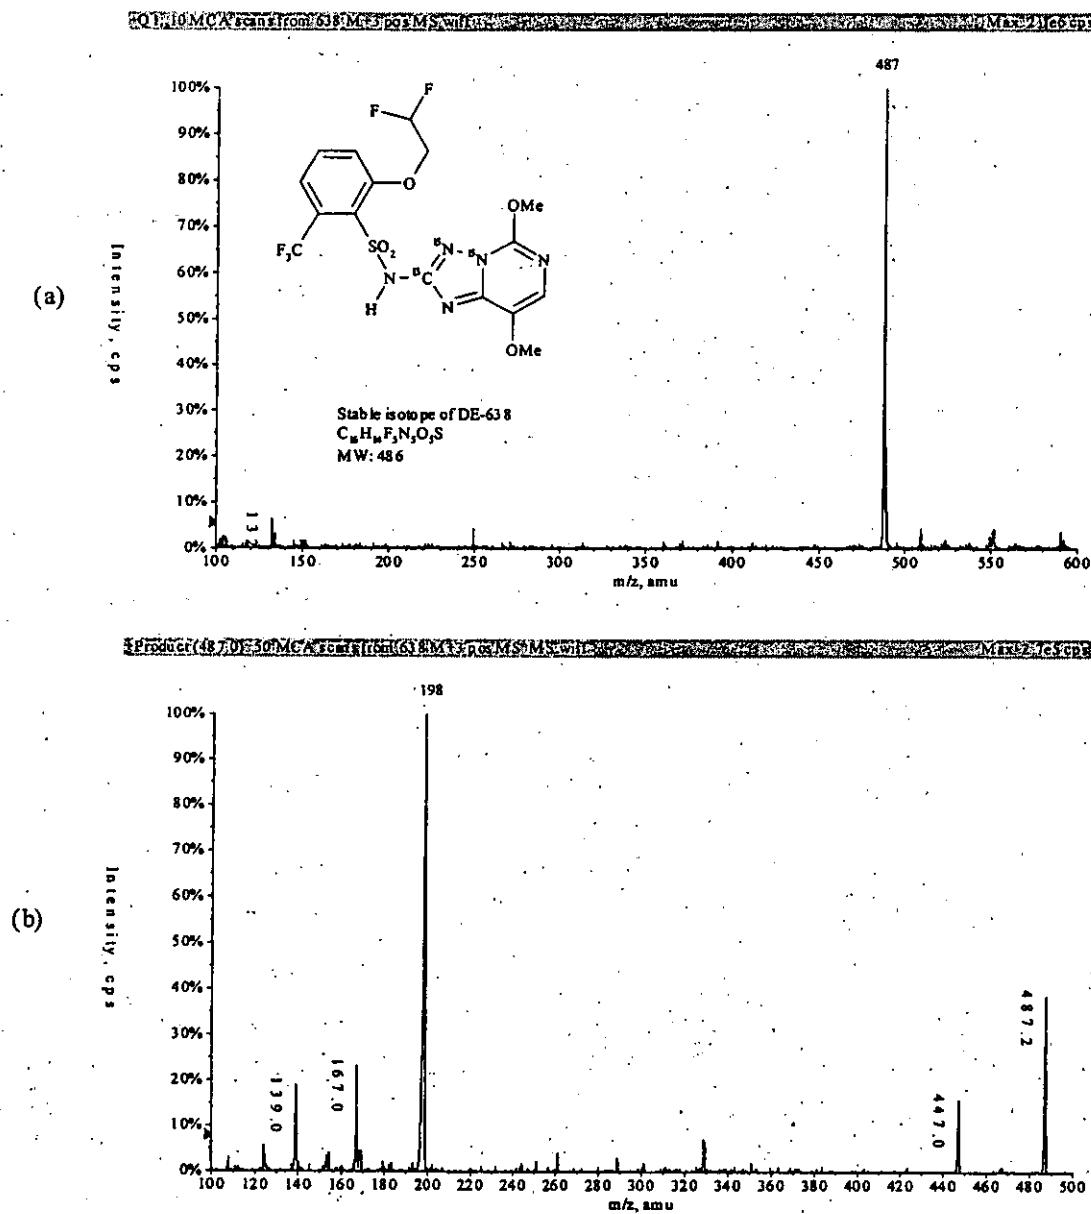



Figure 7. Mass Spectra for XDE-638 M+3 Stable Isotope: (a) Mass Spectrum for Q1 Scan using Electrospray Positive Ionization ($M+H$)⁺ at m/z 487 (b) Product-Ion Mass Spectrum of XDE-638 M+3 Stable Isotope Showing Fragment Ion at m/z 198

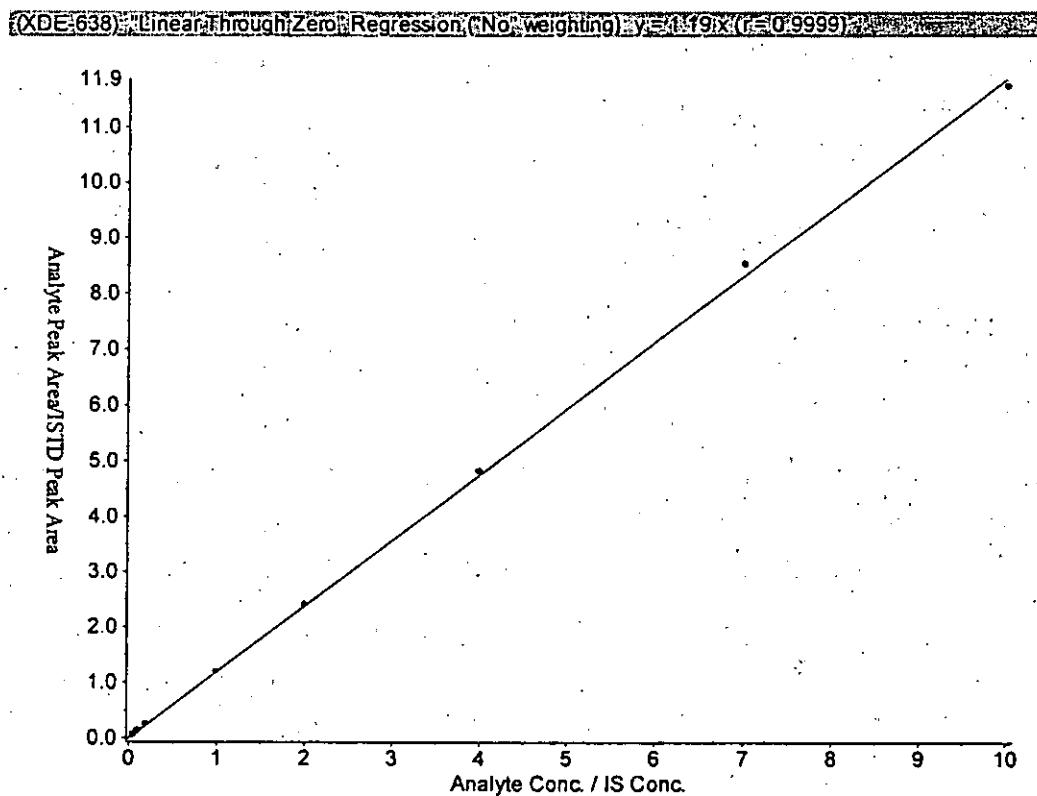

Linear Equation: $Y = 1.19X$
Correlation Coefficient (r): 0.9999
Weighting: none, forced through zero

XDE-638 Conc./ ISTD Conc.	Equivalent Sample Conc. ng/g	XDE-638/ISTD Quantitation Ratio 484/487 amu
0.05	1.3	0.0589
0.1	2.7	0.1176
0.2	5.3	0.2478
1.0	26.7	1.1849
2.0	53.3	2.3828
4.0	106.7	4.8031
7.0	186.7	8.5106
10.0	266.7	11.7269


Figure 8. Typical Calibration Curve for the Determination of XDE-638 in Soil and Sediment

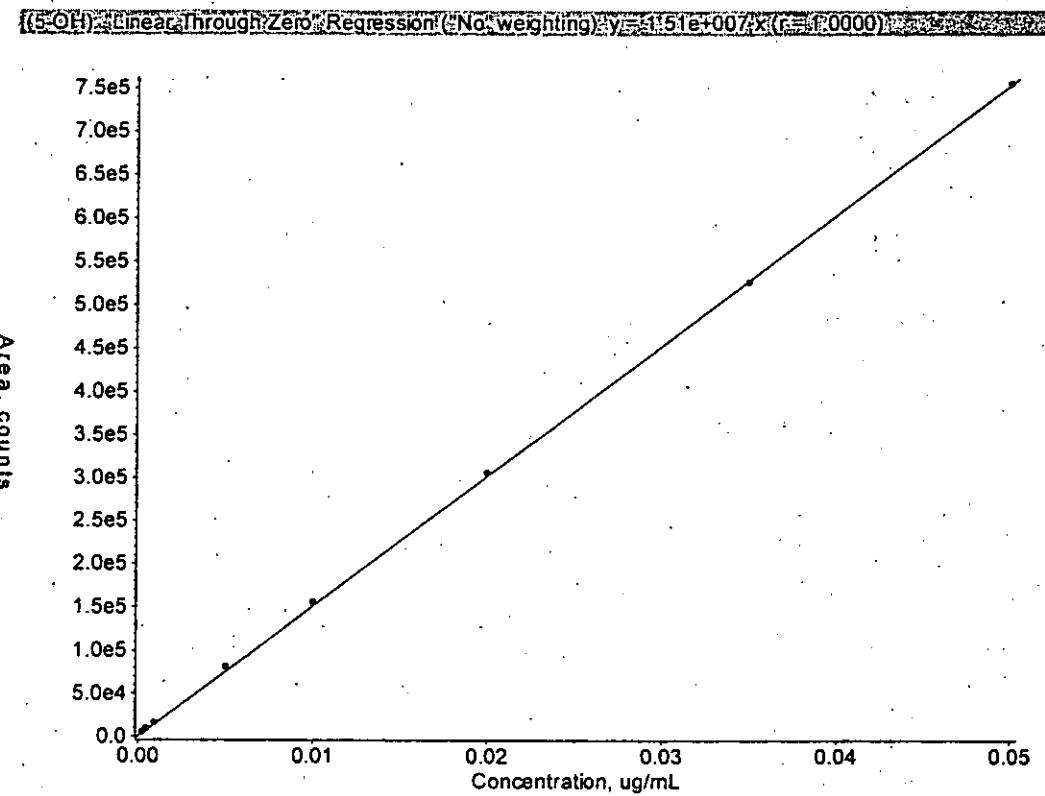

Linear Equation: $Y = 1.51e7X$
Correlation Coefficient (r): 1.0000
Weighting: none, forced through zero

5-OH Metabolite Conc. $\mu\text{g}/\text{mL}$	Equivalent Sample Conc. ng/g	5-OH metabolite of XDE-638 Peak Area
0.00025	1.3	4.25e3
0.0005	2.7	8.00e3
0.001	5.3	1.50e4
0.005	26.7	8.08e4
0.01	53.3	1.54e5
0.02	106.7	3.04e5
0.035	186.7	5.26e5
0.05	266.7	7.55e5


Figure 9. Typical Calibration Curve for the Determination of the 5-OH Metabolite of XDE-638 in Soil and Sediment

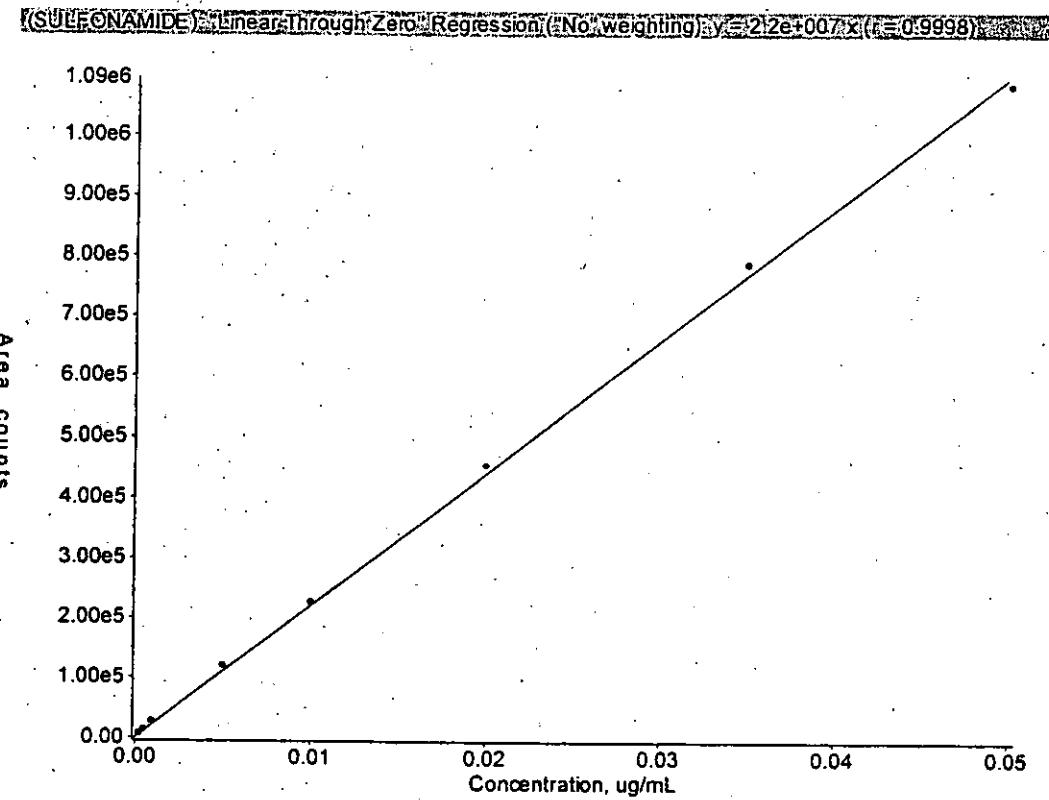

Linear Equation: $Y = 2.2e7X$
Correlation Coefficient (r): 0.9998
Weighting: none, forced through zero

Sulfonamide Metabolite Conc. μg/mL	Equivalent Sample Conc. ng/g	Sulfonamide metabolite of XDE-638 Peak Area
0.00025	1.3	6.77e3
0.0005	2.7	1.35e4
0.001	5.3	2.64e4
0.005	26.7	1.18e5
0.01	53.3	2.26e5
0.02	106.7	4.52e5
0.035	186.7	7.86e5
0.05	266.7	1.08e6


Figure 10. Typical Calibration Curve for the Determination of the Sulfonamide Metabolite of XDE-638 in Soil and Sediment

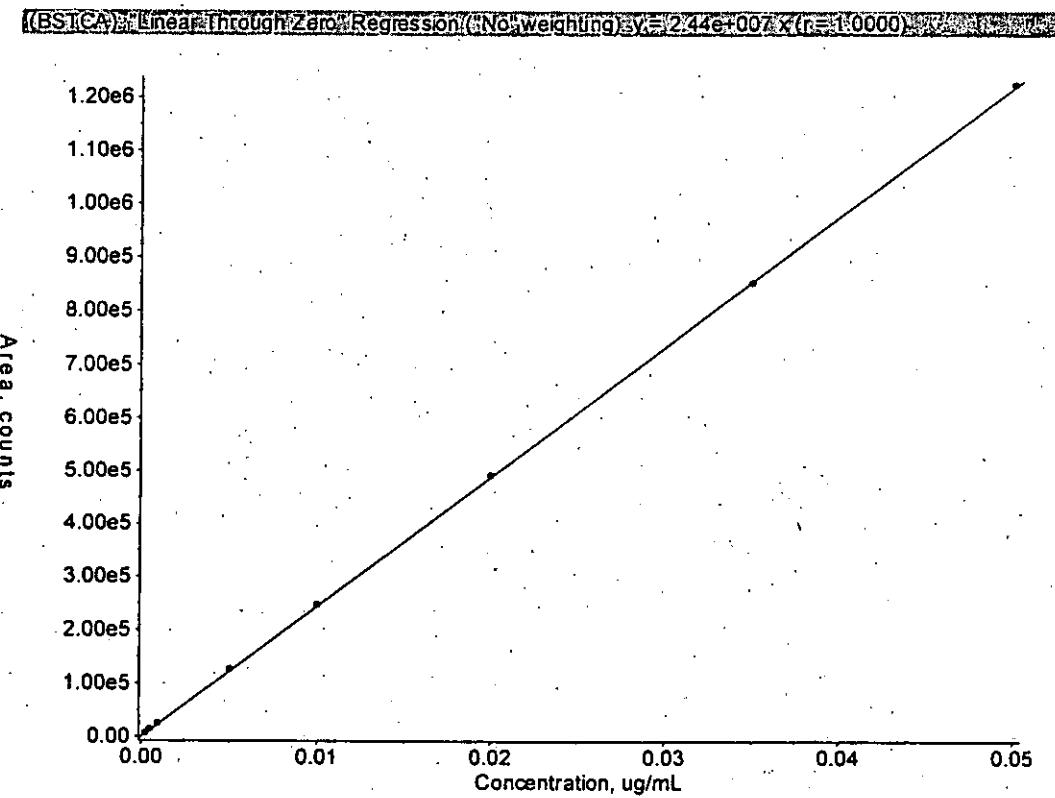

Linear Equation: $Y = 2.44e7X$
Correlation Coefficient (r): 1.0000
Weighting: none, forced through zero

BSTCA Metabolite Conc. ug/mL	Equivalent Sample Conc. ng/g	BSTCA metabolite of XDE-638 Peak Area
0.00025	1.3	5.92e3
0.0005	2.7	1.22e4
0.001	5.3	2.42e4
0.005	26.7	1.25e5
0.01	53.3	2.46e5
0.02	106.7	4.91e5
0.035	186.7	8.51e5
0.05	266.7	1.22e6


Figure 11. Typical Calibration Curve for the Determination of the BSTCA Metabolite of XDE-638 in Soil and Sediment

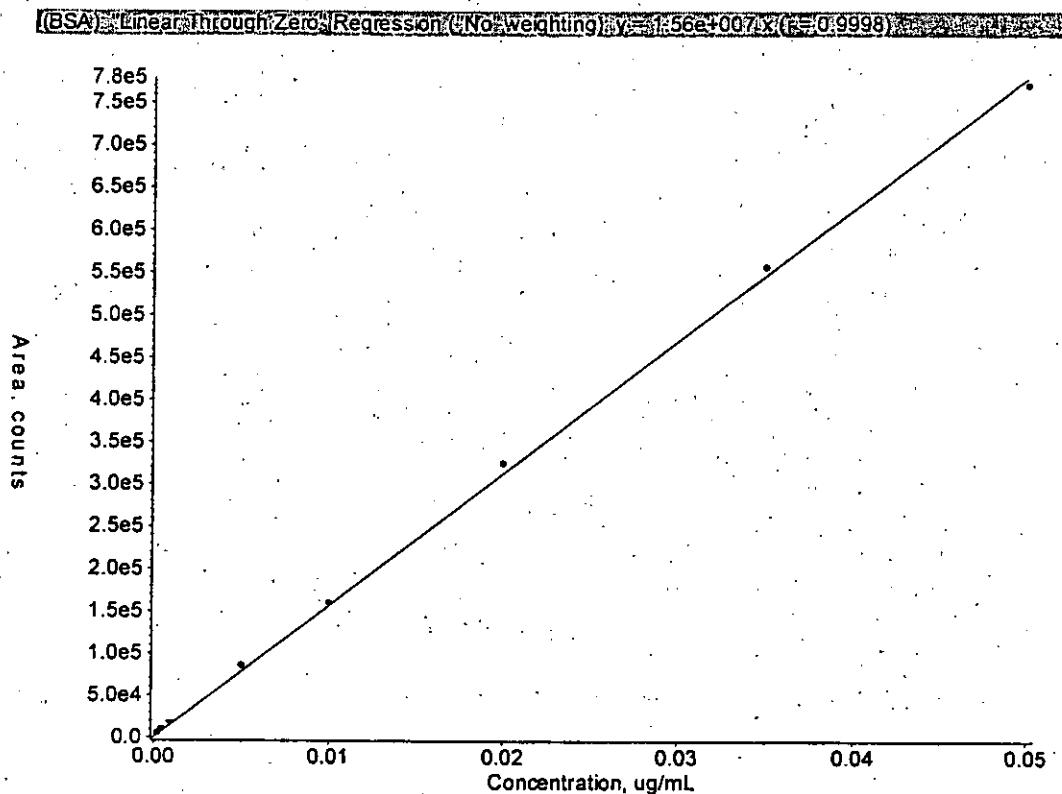

Linear Equation: $Y = 1.56e7X$
Correlation Coefficient (r): 0.9998
Weighting: none, forced through zero

BSA Metabolite Conc. μg/mL	Equivalent Sample Conc. ng/g	BSA metabolite of XDE-638 Peak Area
0.00025	1.3	4.84e3
0.0005	2.7	8.87e3
0.001	5.3	1.73e4
0.005	26.7	8.41e4
0.01	53.3	1.59e5
0.02	106.7	3.23e5
0.035	186.7	5.55e5
0.05	266.7	7.71e5

Figure 12. Typical Calibration Curve for the Determination of the BSA Metabolite of XDE-638 in Soil and Sediment

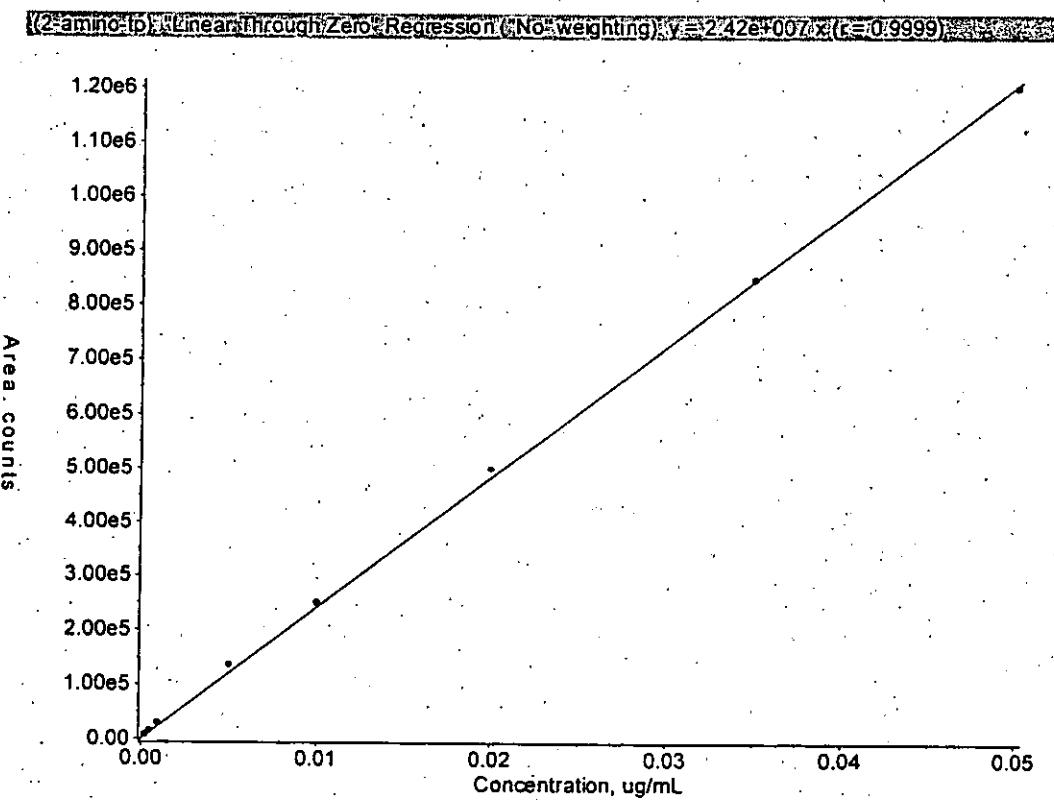

Linear Equation: $Y = 2.42e7X$
Correlation Coefficient (r): 0.9999
Weighting: none, forced through zero

2-Amino-TP Metabolite Conc. μg/mL	Equivalent Sample Conc. ng/g	2-Amino-TP metabolite of XDE-638 Peak Area
0.00025	1.3	7.10e3
0.0005	2.7	1.29e4
0.001	5.3	2.72e4
0.005	26.7	1.35e5
0.01	53.3	2.50e5
0.02	106.7	4.98e5
0.035	186.7	8.45e5
0.05	266.7	1.20e6

Figure 13. Typical Calibration Curve for the Determination of the 2-Amino-TP Metabolite of XDE-638 in Soil and Sediment

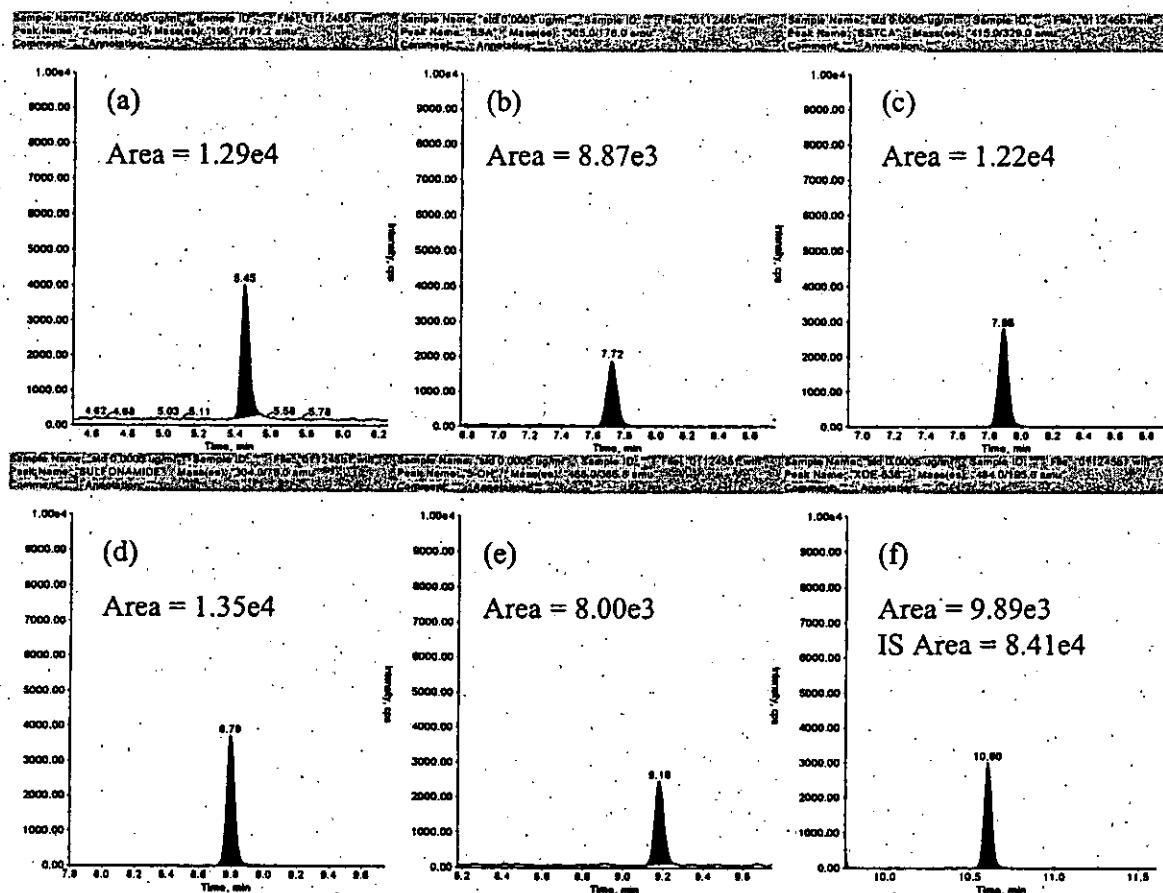


Figure 14. Typical MRM Chromatograms for the Determination of XDE-638 and Metabolites in Soil and Sediment

0.0005- μ g/mL Standard. Equivalent to a sample concentration of 2.67 ng/g.

- (a) 2-Amino TP Metabolite
- (b) BSA Metabolite
- (c) BSTCA Metabolite
- (d) Sulfonamide Metabolite
- (e) 5-OH Metabolite
- (f) XDE-638

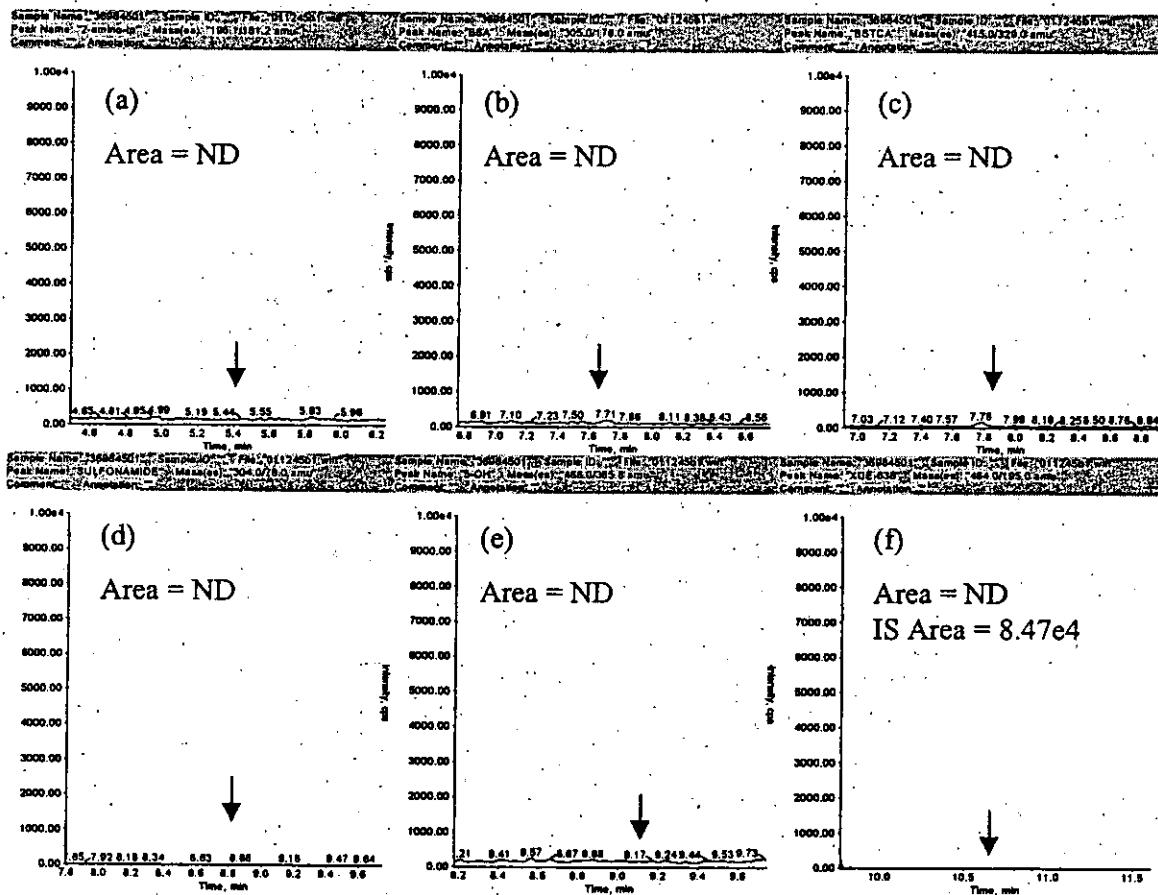


Figure 15. Typical MRM Chromatograms for the Determination of XDE-638 and Metabolites in Soil and Sediment

Control Soil Sample 36984501: No Detectable (ND) Residue of XDE-638 and metabolites.

- (a) 2-Amino TP Metabolite
- (b) BSA Metabolite
- (c) BSTCA Metabolite
- (d) Sulfonamide Metabolite
- (e) 5-OH Metabolite
- (f) XDE-638

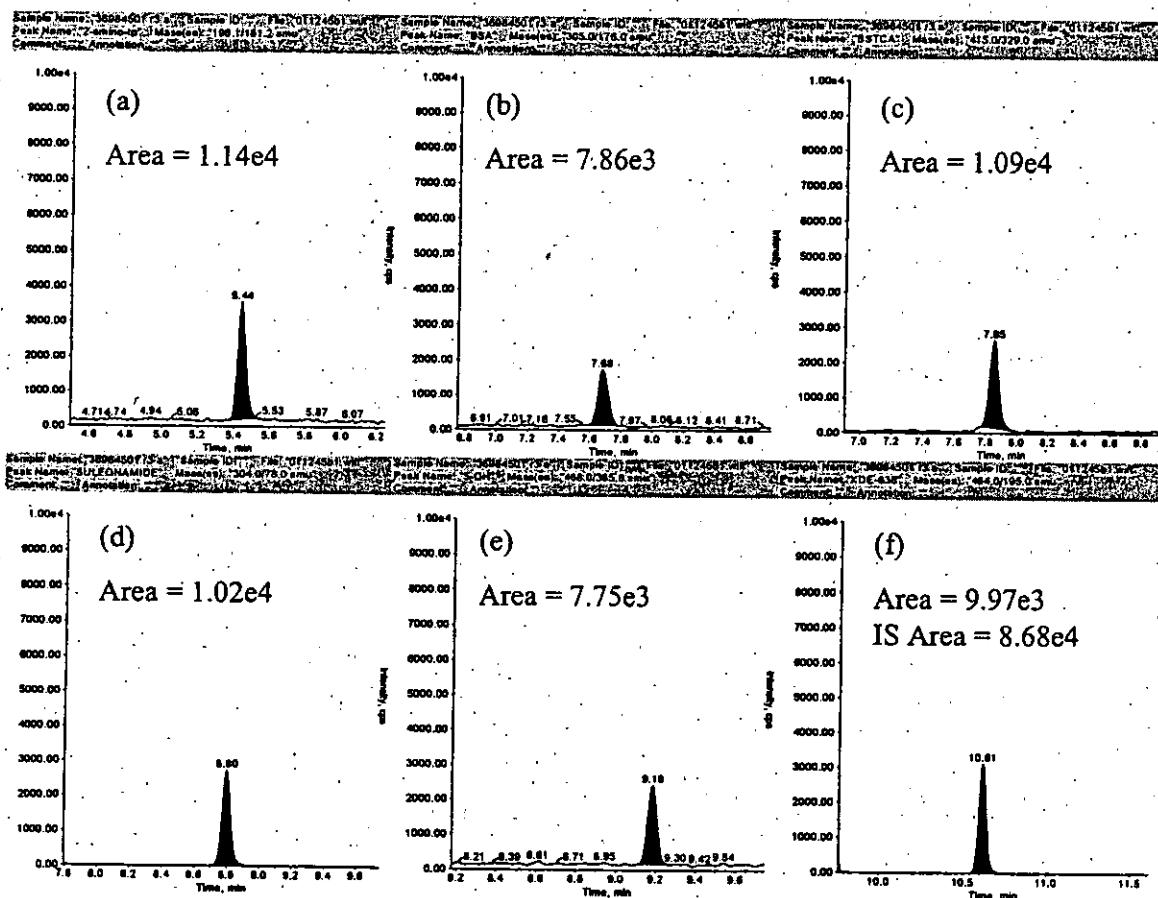


Figure 16. Typical MRM Chromatograms for the Determination of XDE-638 and Metabolites in Soil and Sediment

Control Soil Sample 36984501 Fortified at 3 ng/g.

- (a) 2-Amino TP Metabolite; 84% Recovery
- (b) BSA Metabolite; 89% Recovery
- (c) BSTCA Metabolite; 79% Recovery
- (d) Sulfonamide Metabolite; 83% Recovery
- (e) 5-OH Metabolite; 91% Recovery
- (f) XDE-638; 84% Recovery

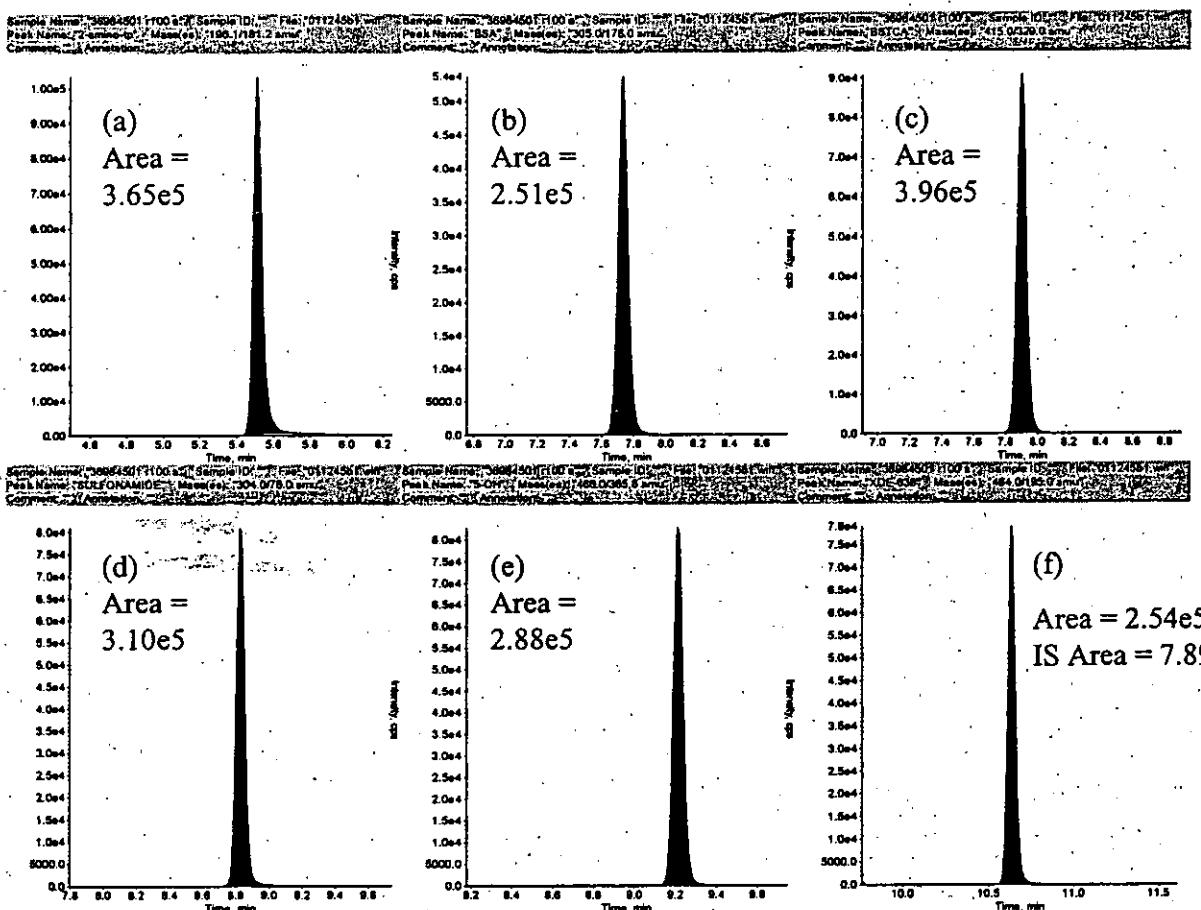


Figure 17. Typical MRM Chromatograms for the Determination of XDE-638 and Metabolites in Soil and Sediment

Control Soil Sample 36984501 Fortified at 100 ng/g.

- (a) 2-Amino TP Metabolite; 81% Recovery
- (b) BSA Metabolite; 86% Recovery
- (c) BSTCA Metabolite; 86% Recovery
- (d) Sulfonamide Metabolite; 75% Recovery
- (e) 5-OH Metabolite; 102% Recovery
- (f) XDE-638; 72% Recovery

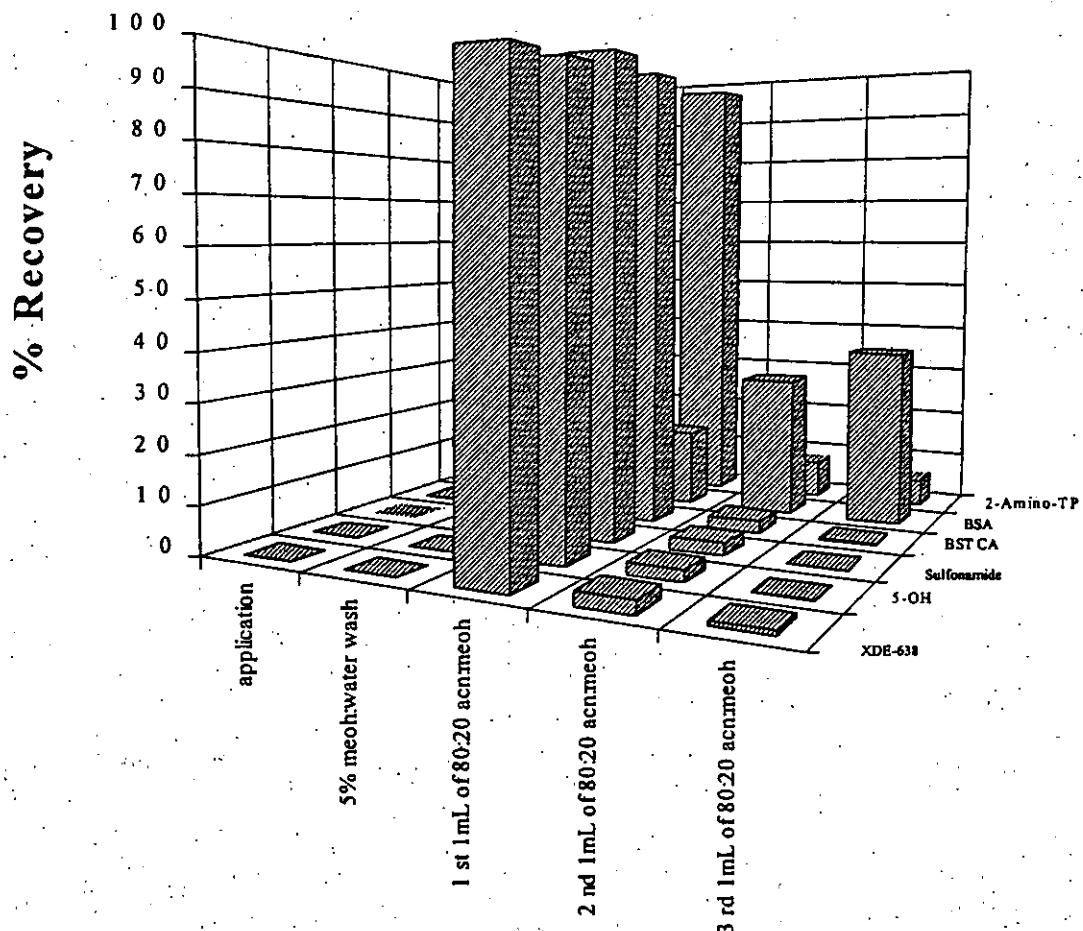


Figure 18. Typical Waters HLB SPE Plate Elution Profiles for XDE-638 and Metabolites

Note: This profile was carried out using a fortified 0.1N Hydrochloric acid solution. Without soil matrix present, elution of the BSA metabolite required more than 3 mL of elution solvent for quantitative elution. However, in the presence of soil matrix, complete elution occurred with 2 mL of elution solvent.